

FIG. 1

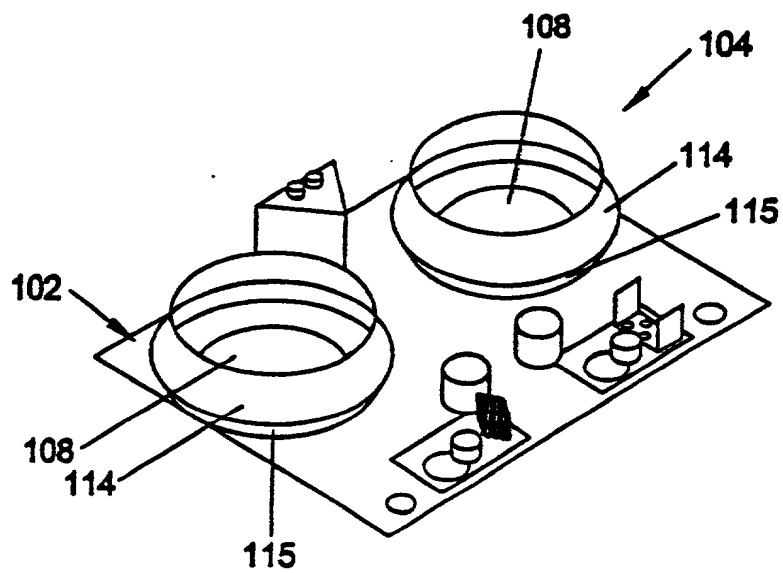


FIG. 2

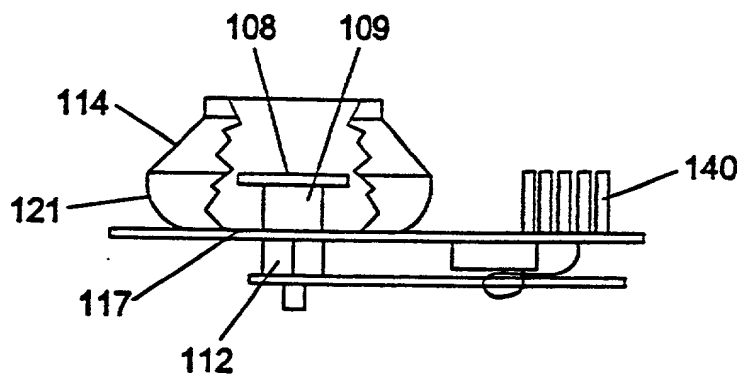


FIG. 3

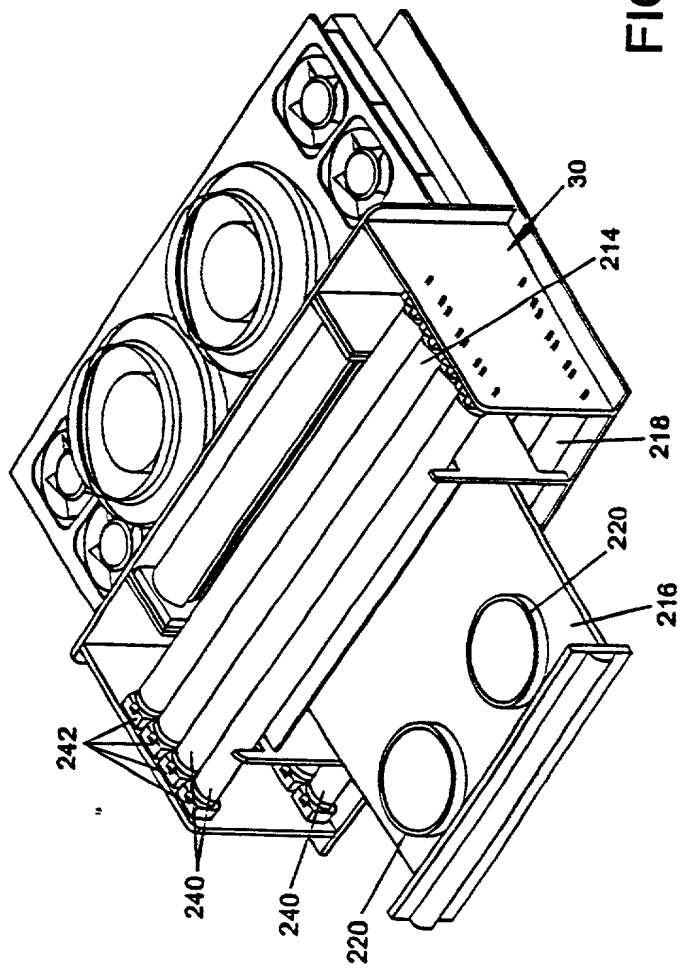


FIG. 4

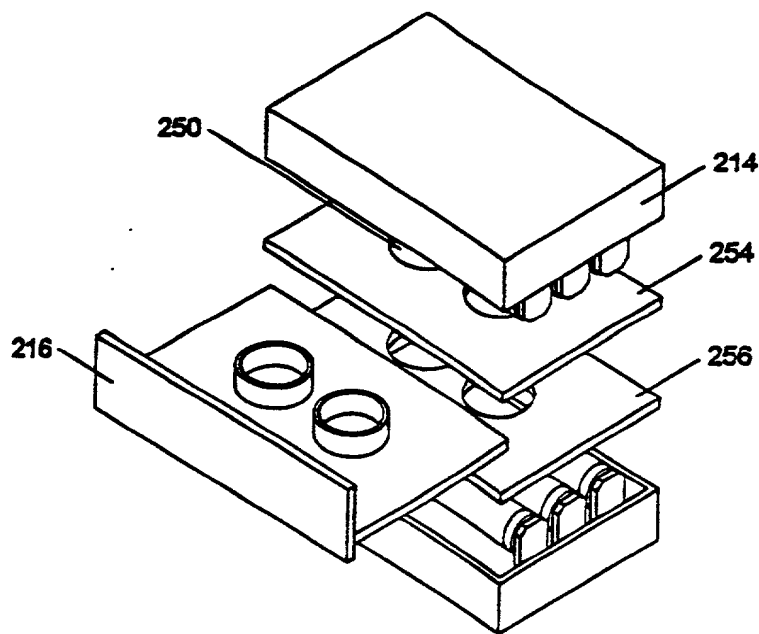


FIG. 5

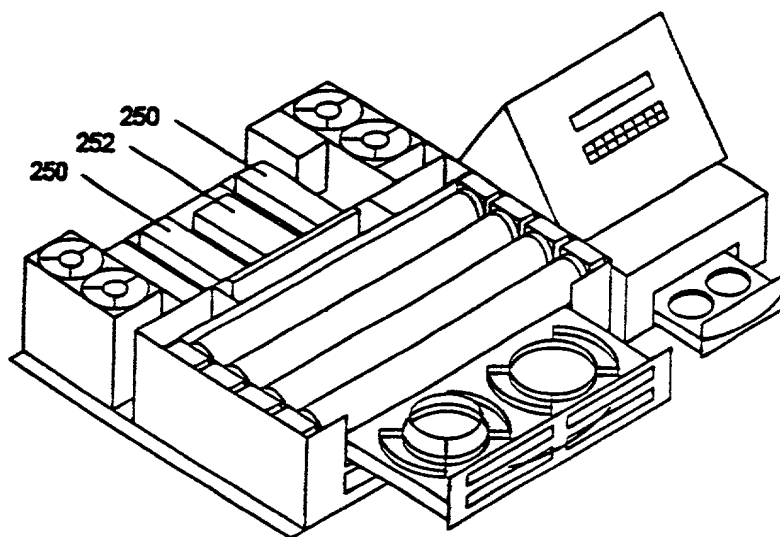


FIG. 6

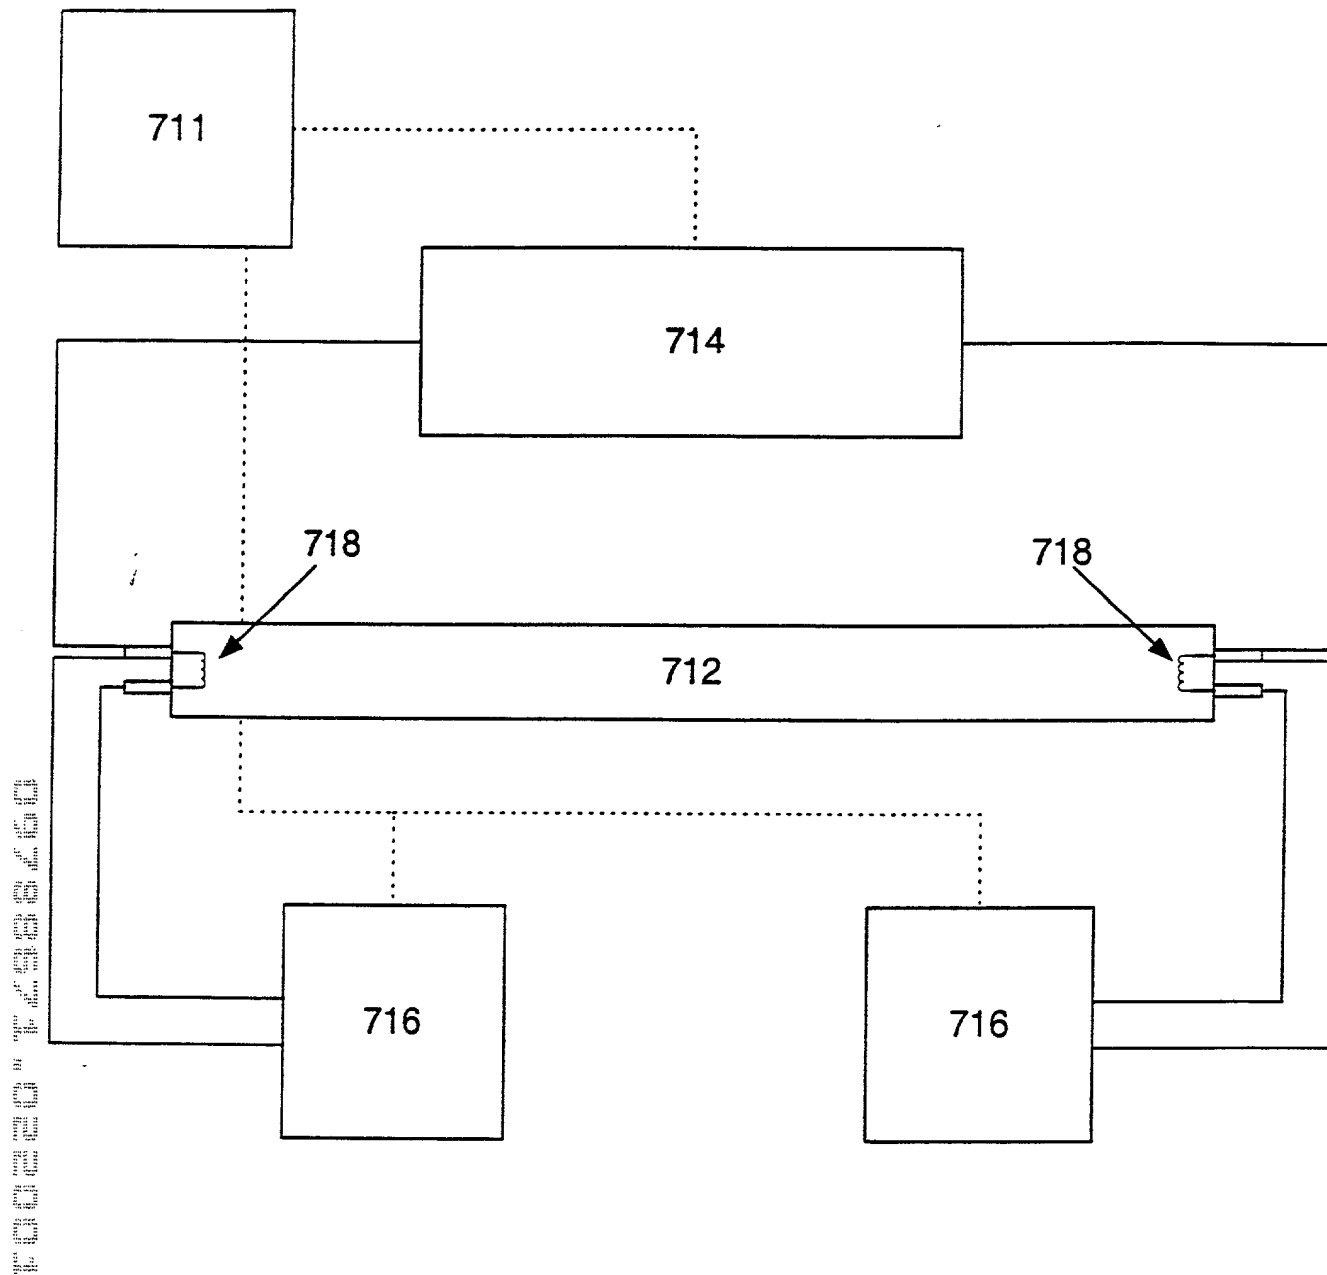


FIG. 7

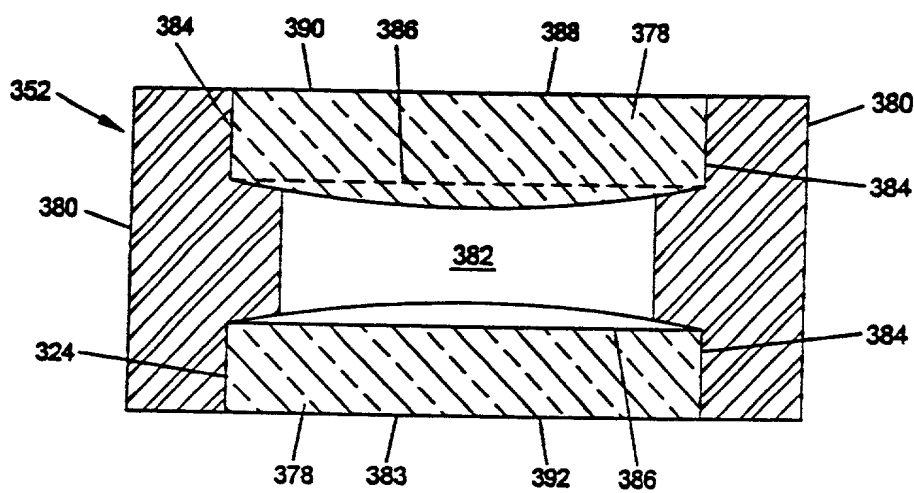


FIG. 8

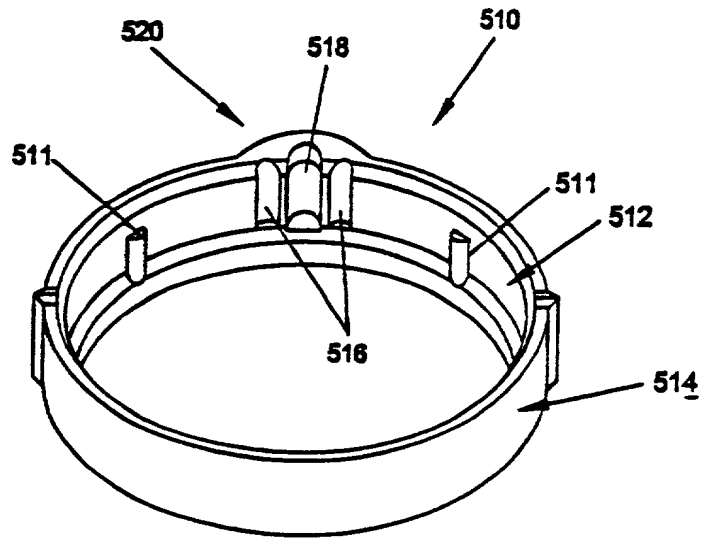


FIG. 9

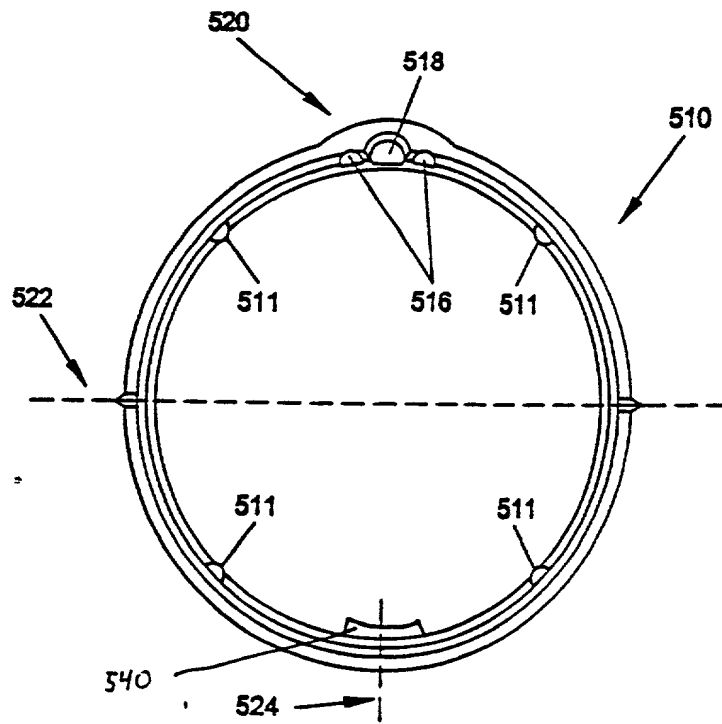


FIG. 10

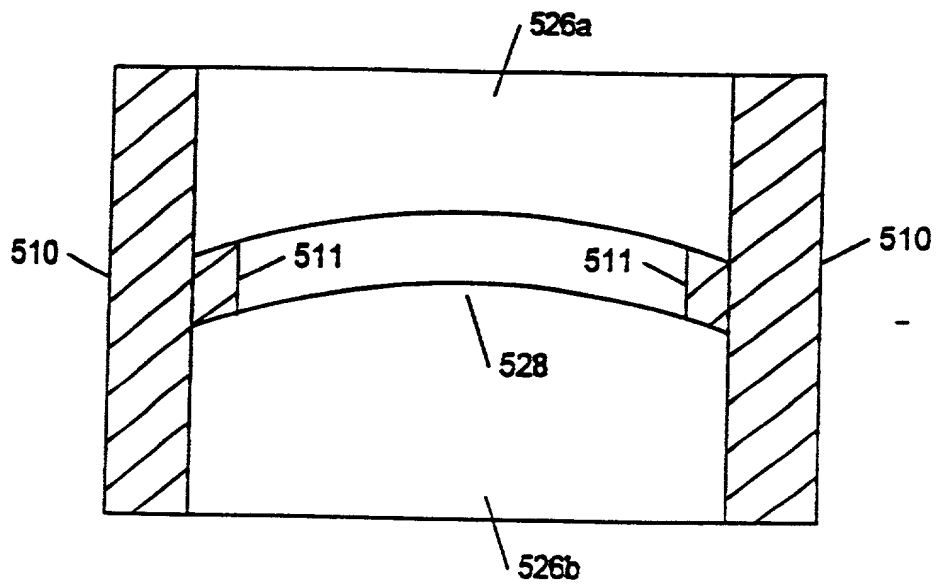


FIG. 11

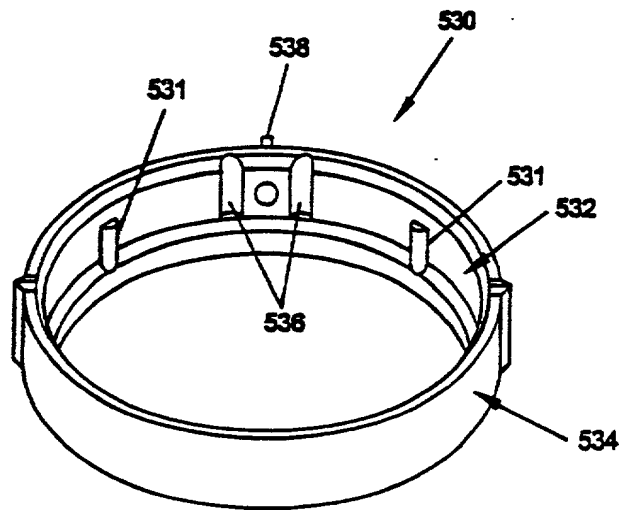


FIG. 12

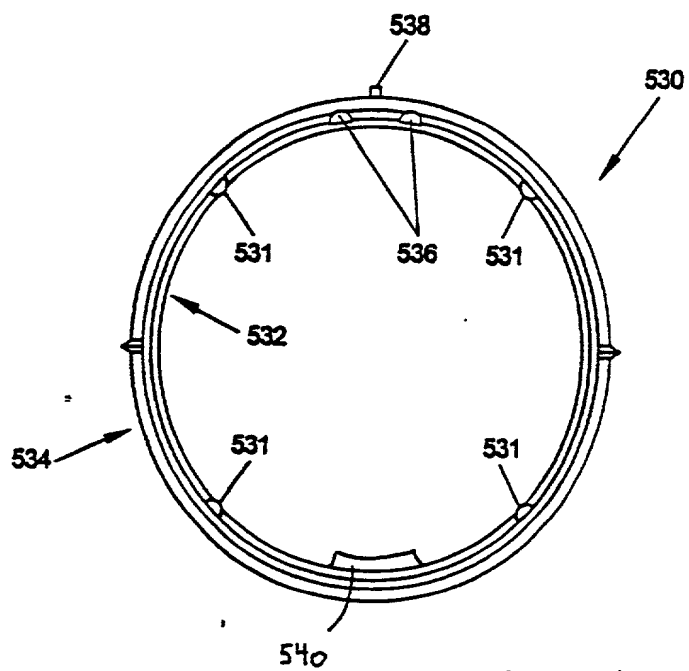


FIG. 13

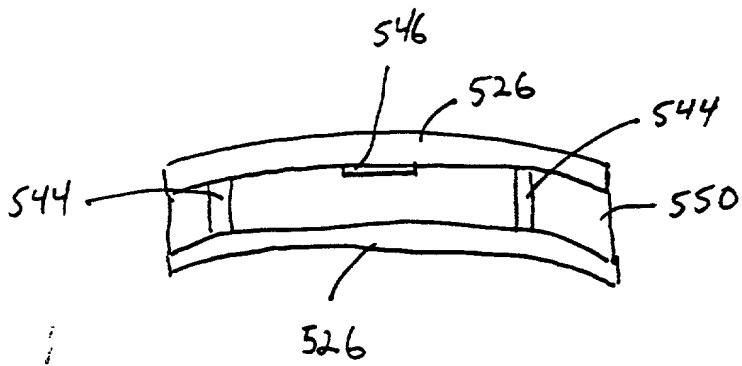


FIG. 14

Downloaded from www.elsevier.com

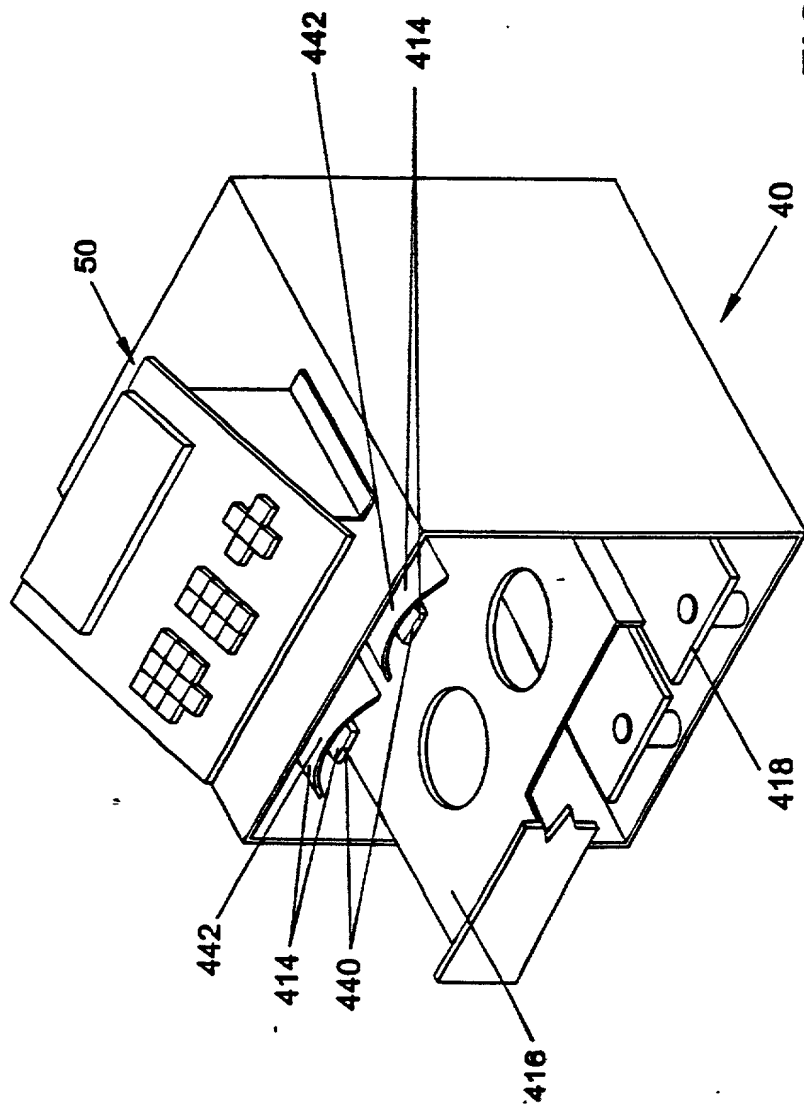


FIG. 15

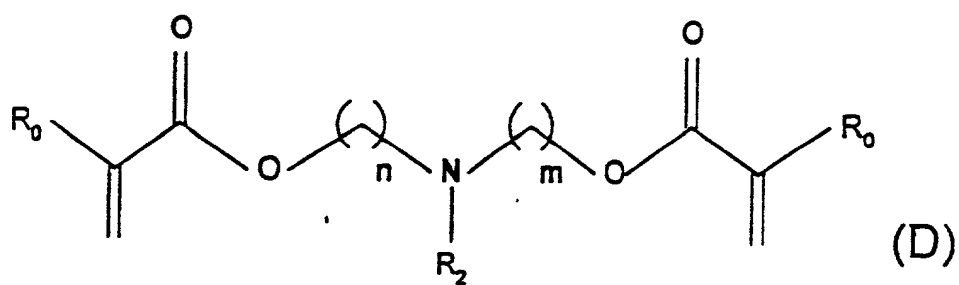
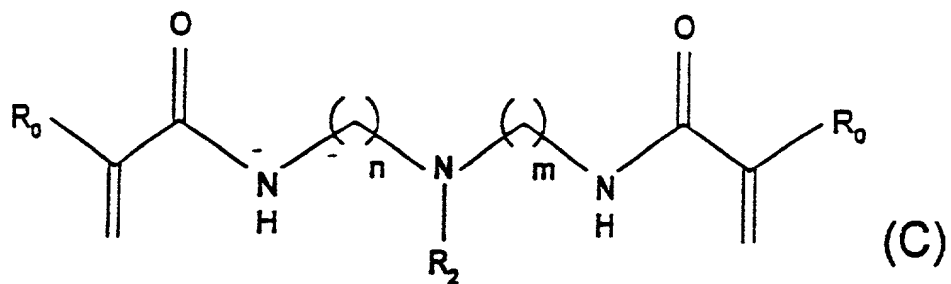
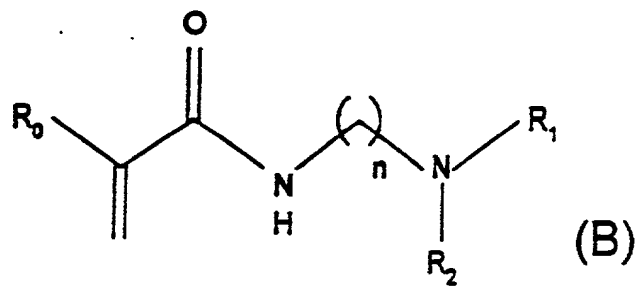
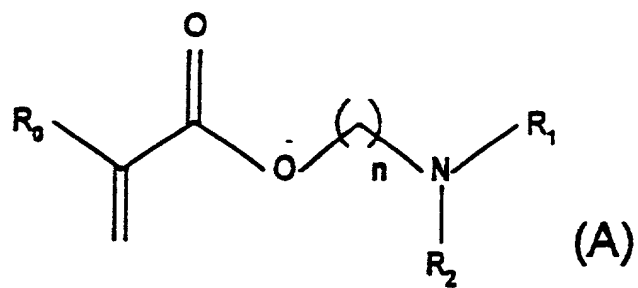


FIG. 16

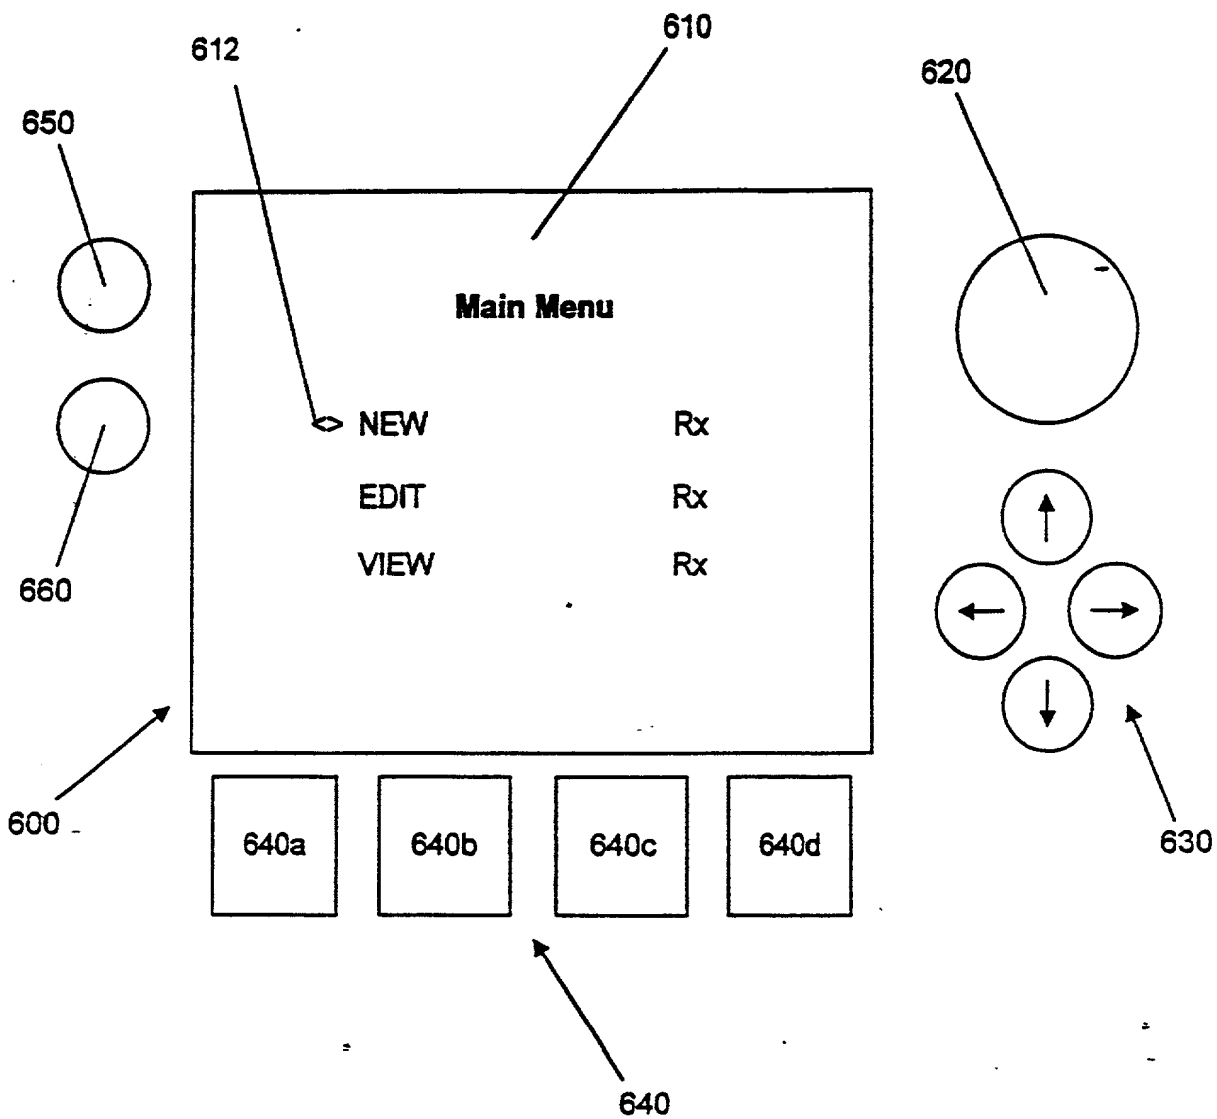


FIG. 17

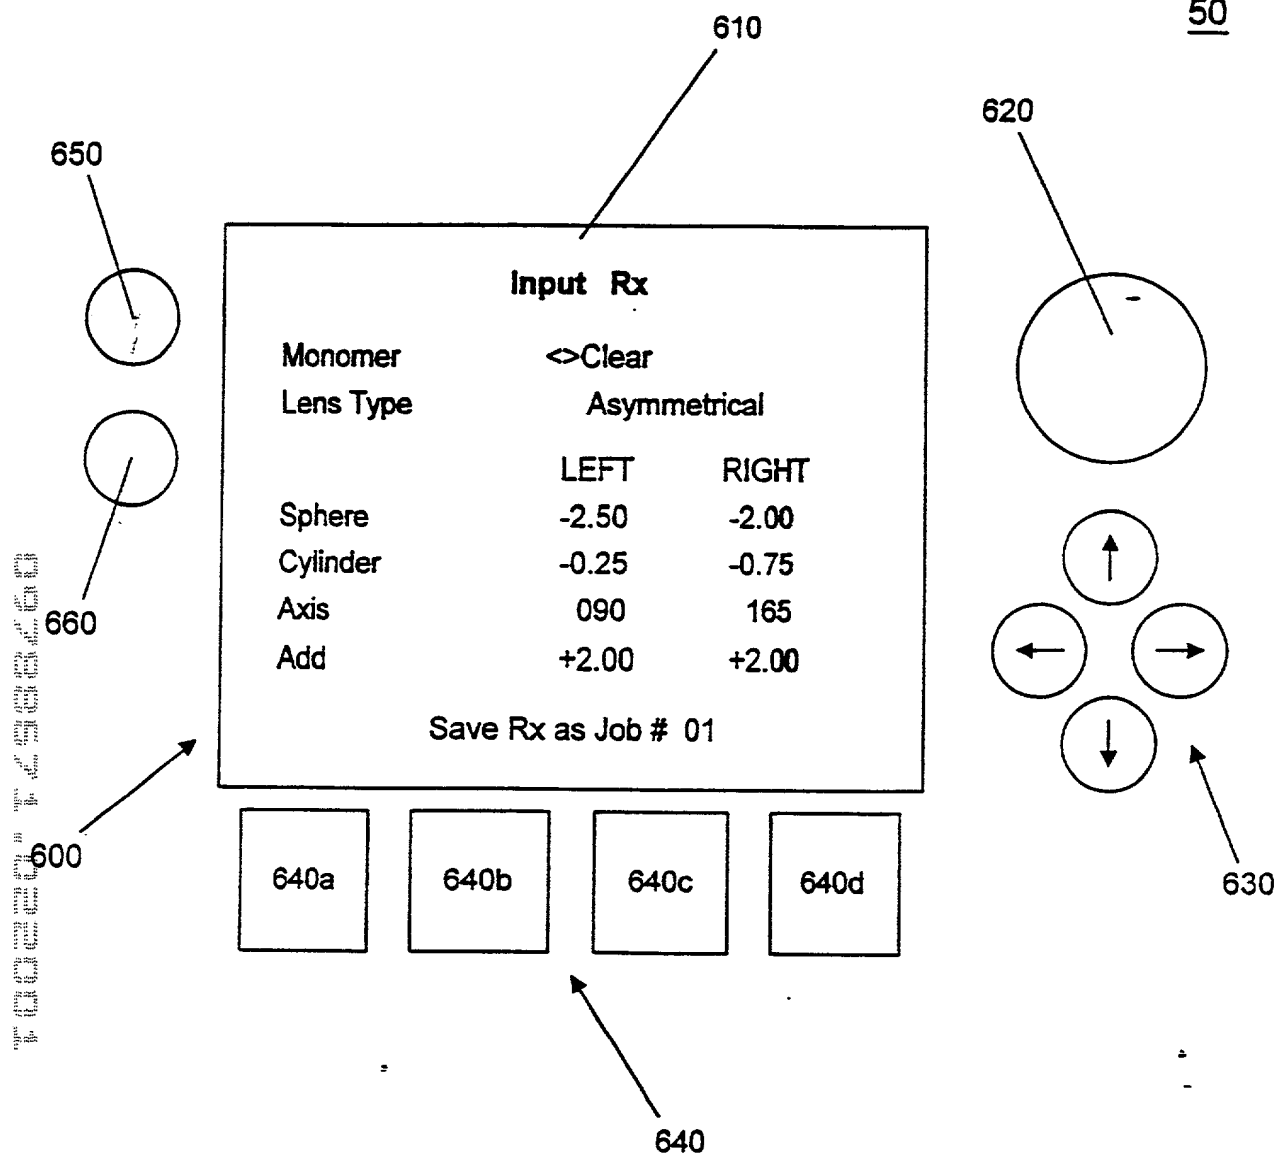


FIG. 18

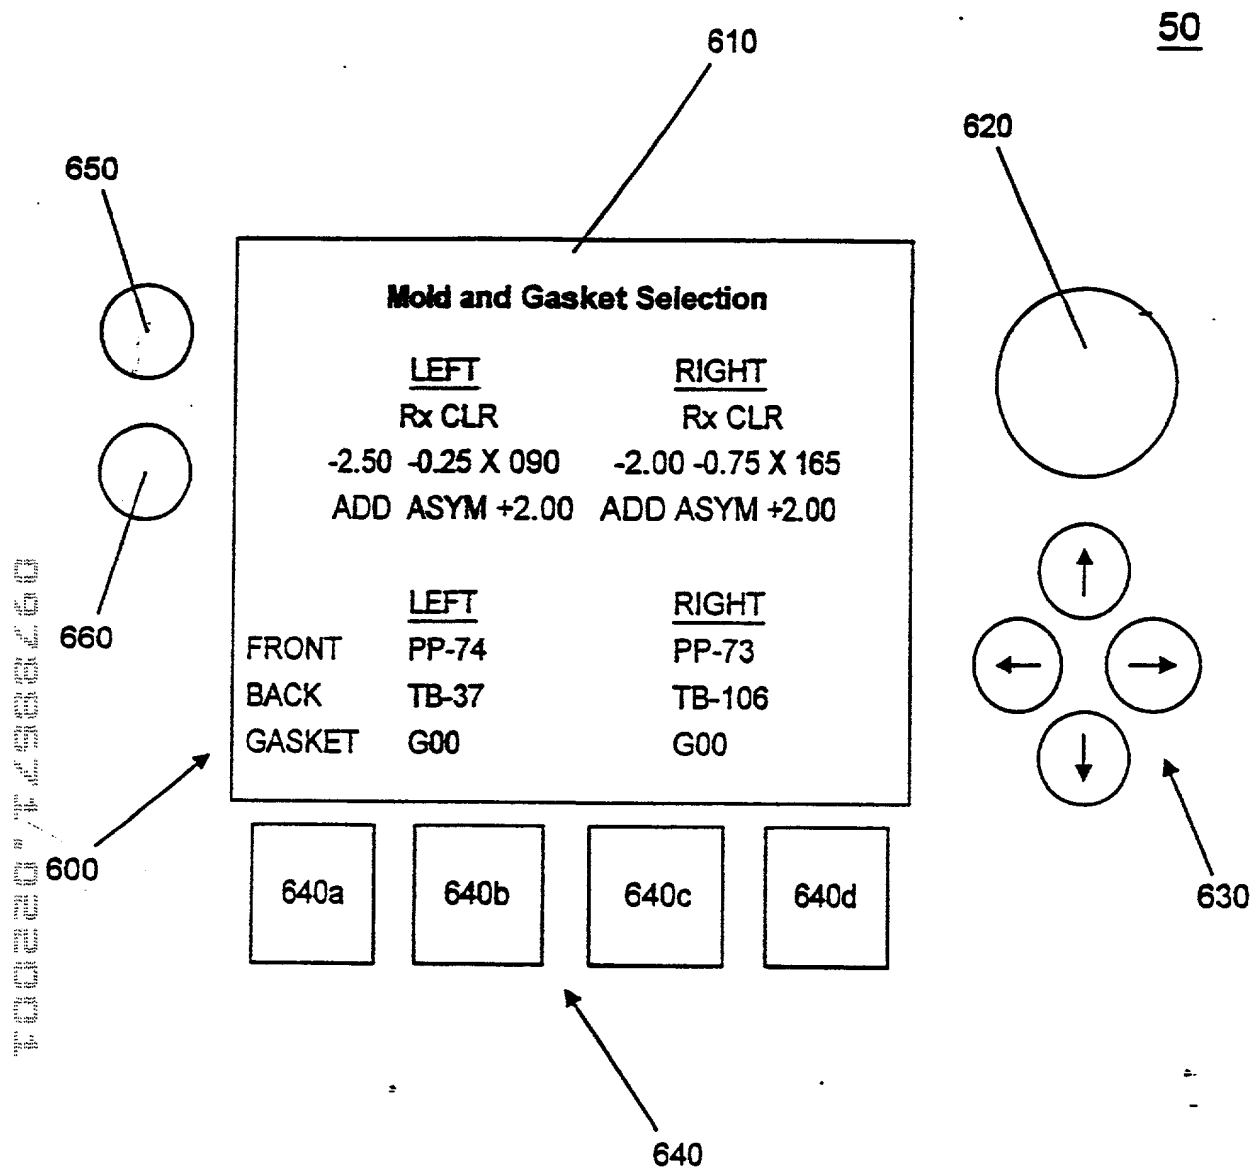
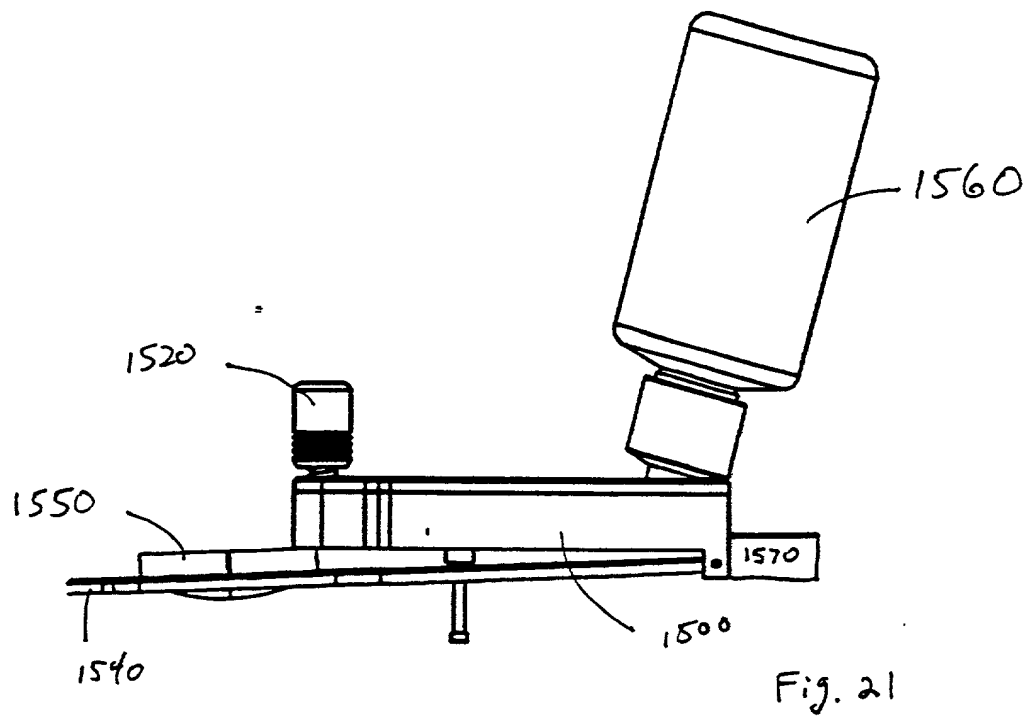
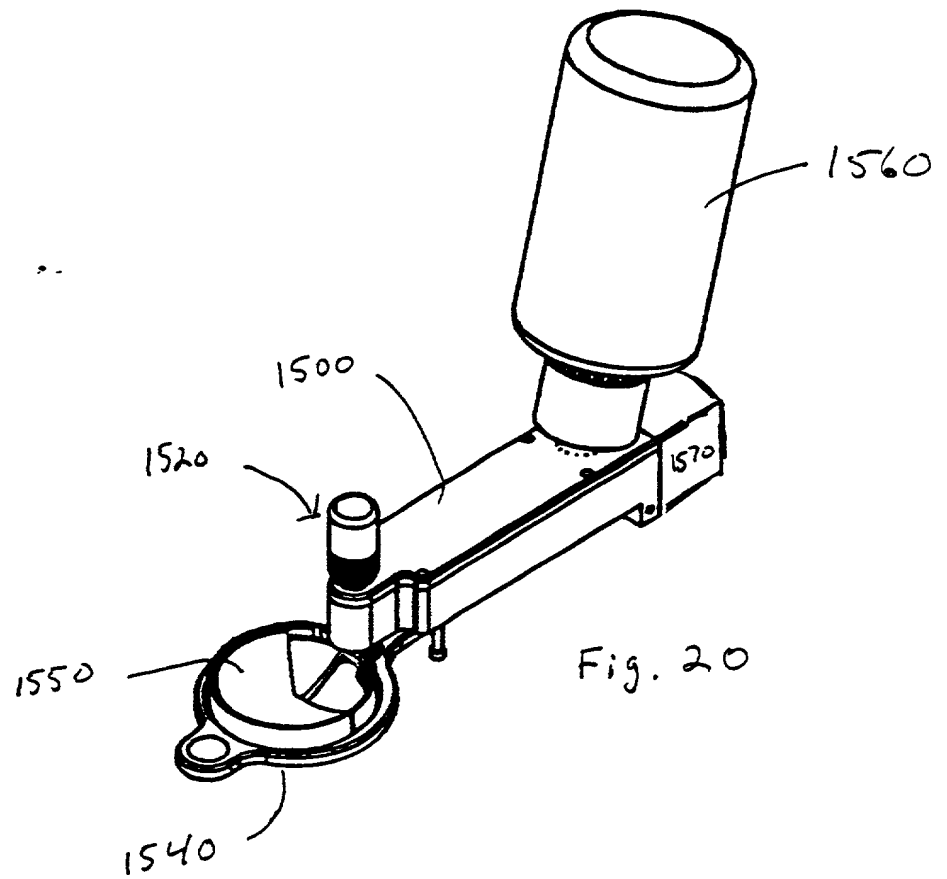
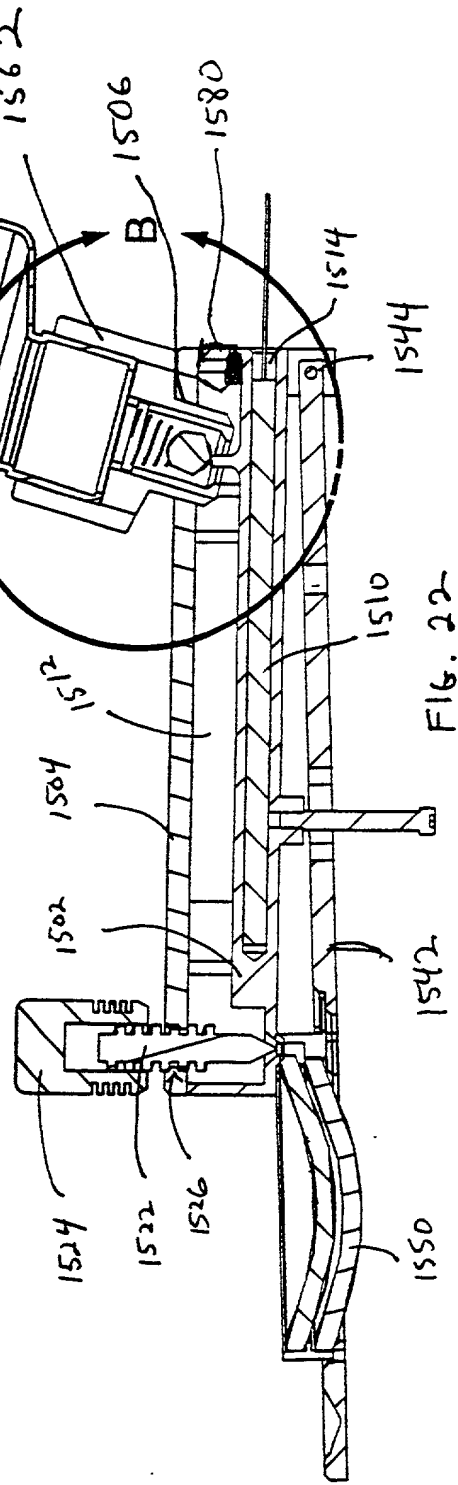
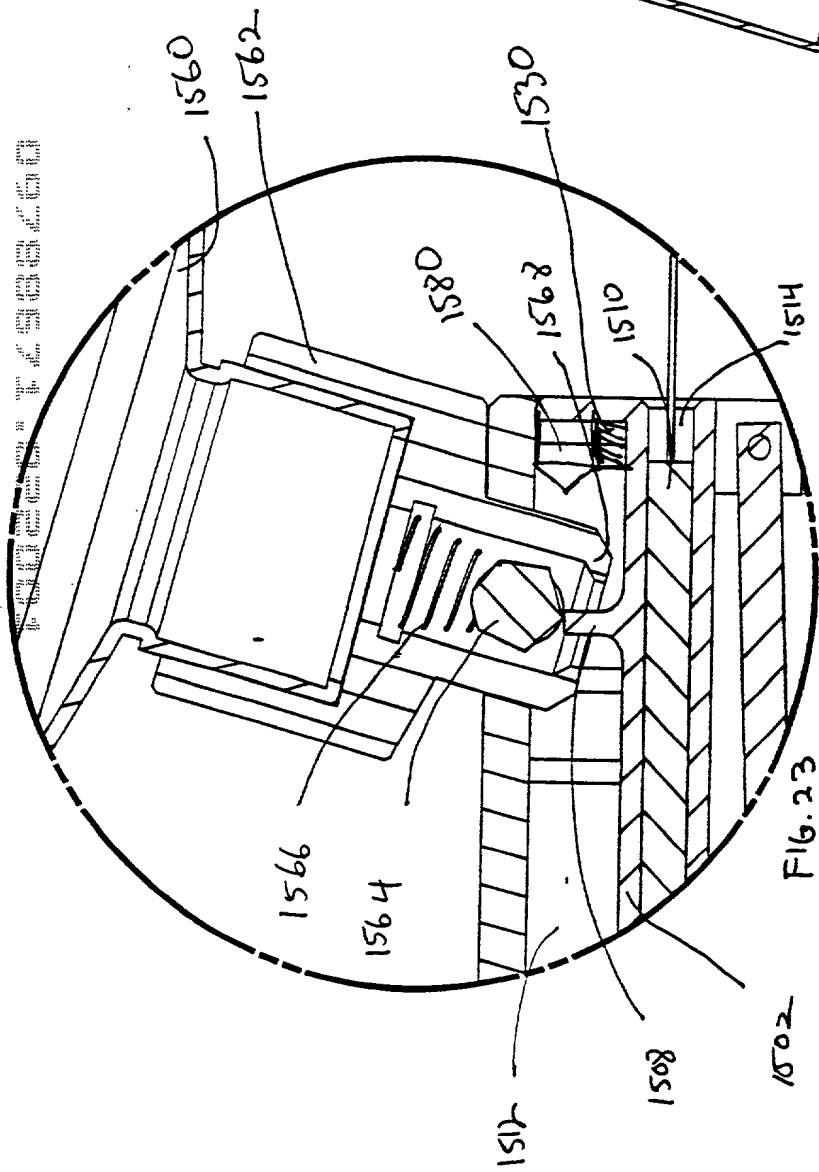


FIG. 19





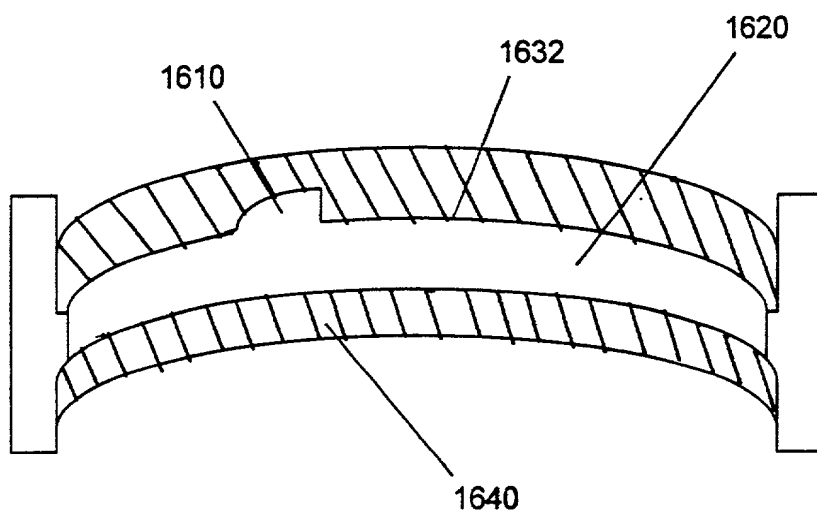


FIG. 24

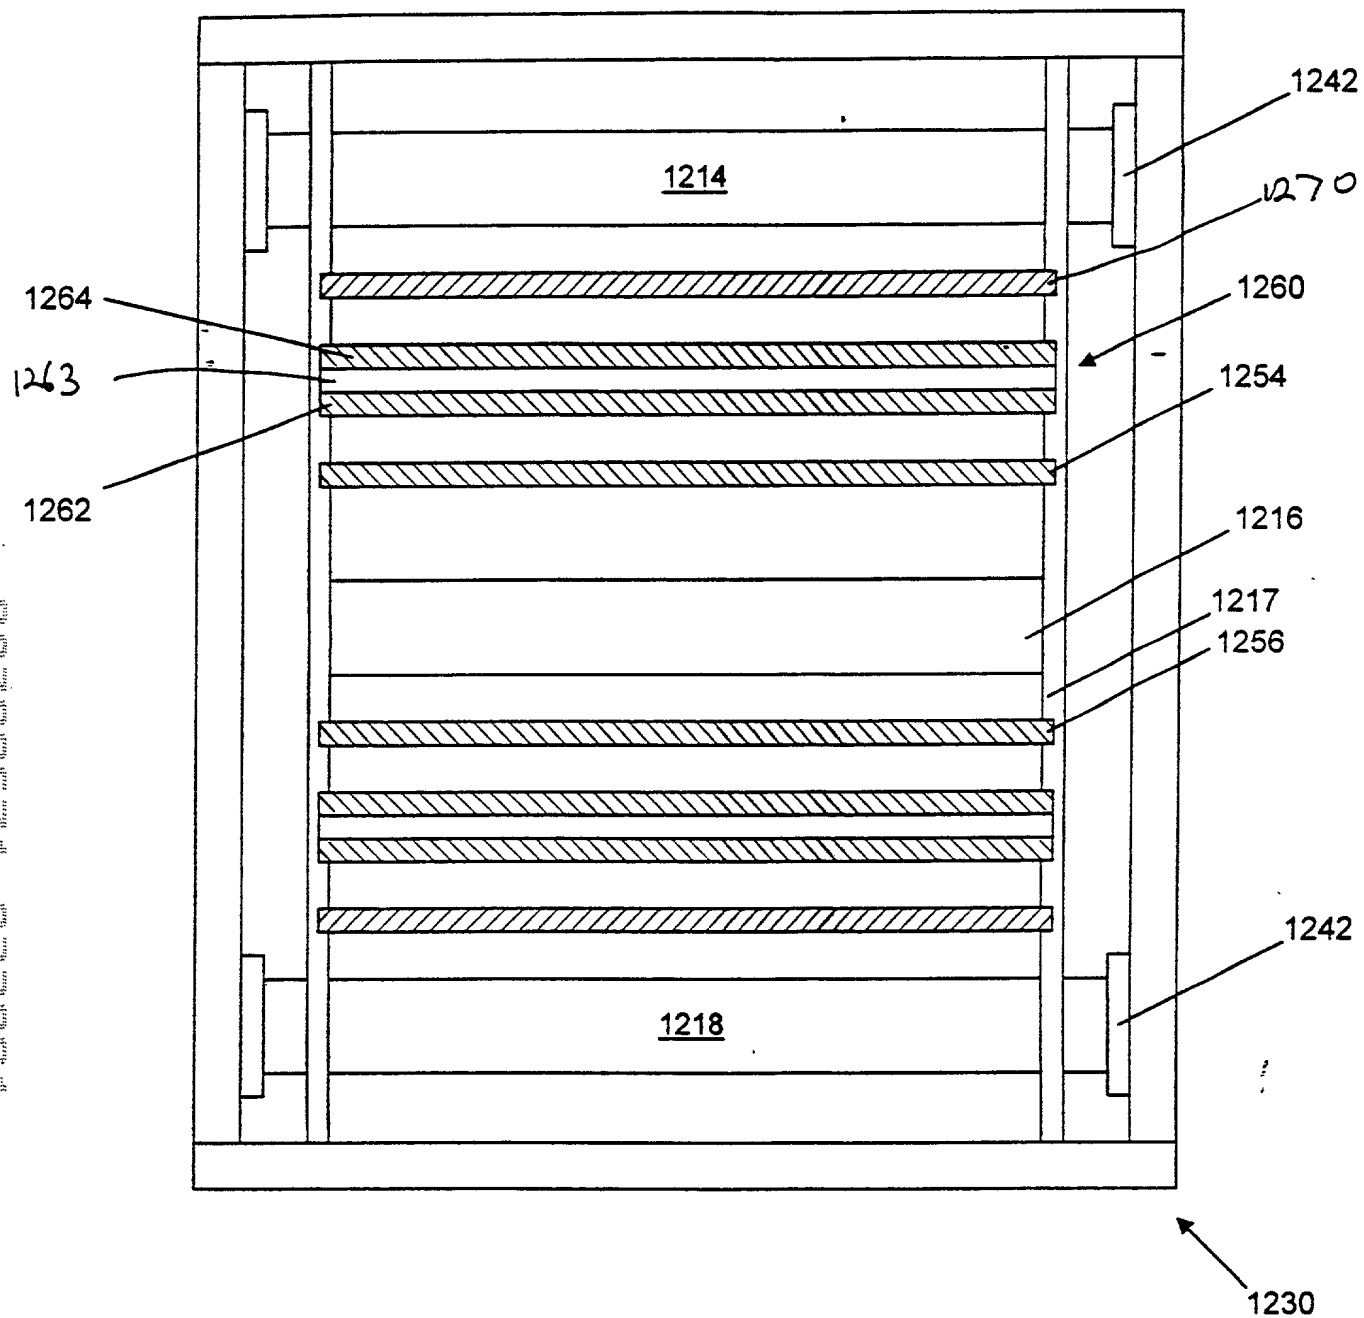


FIG. 25

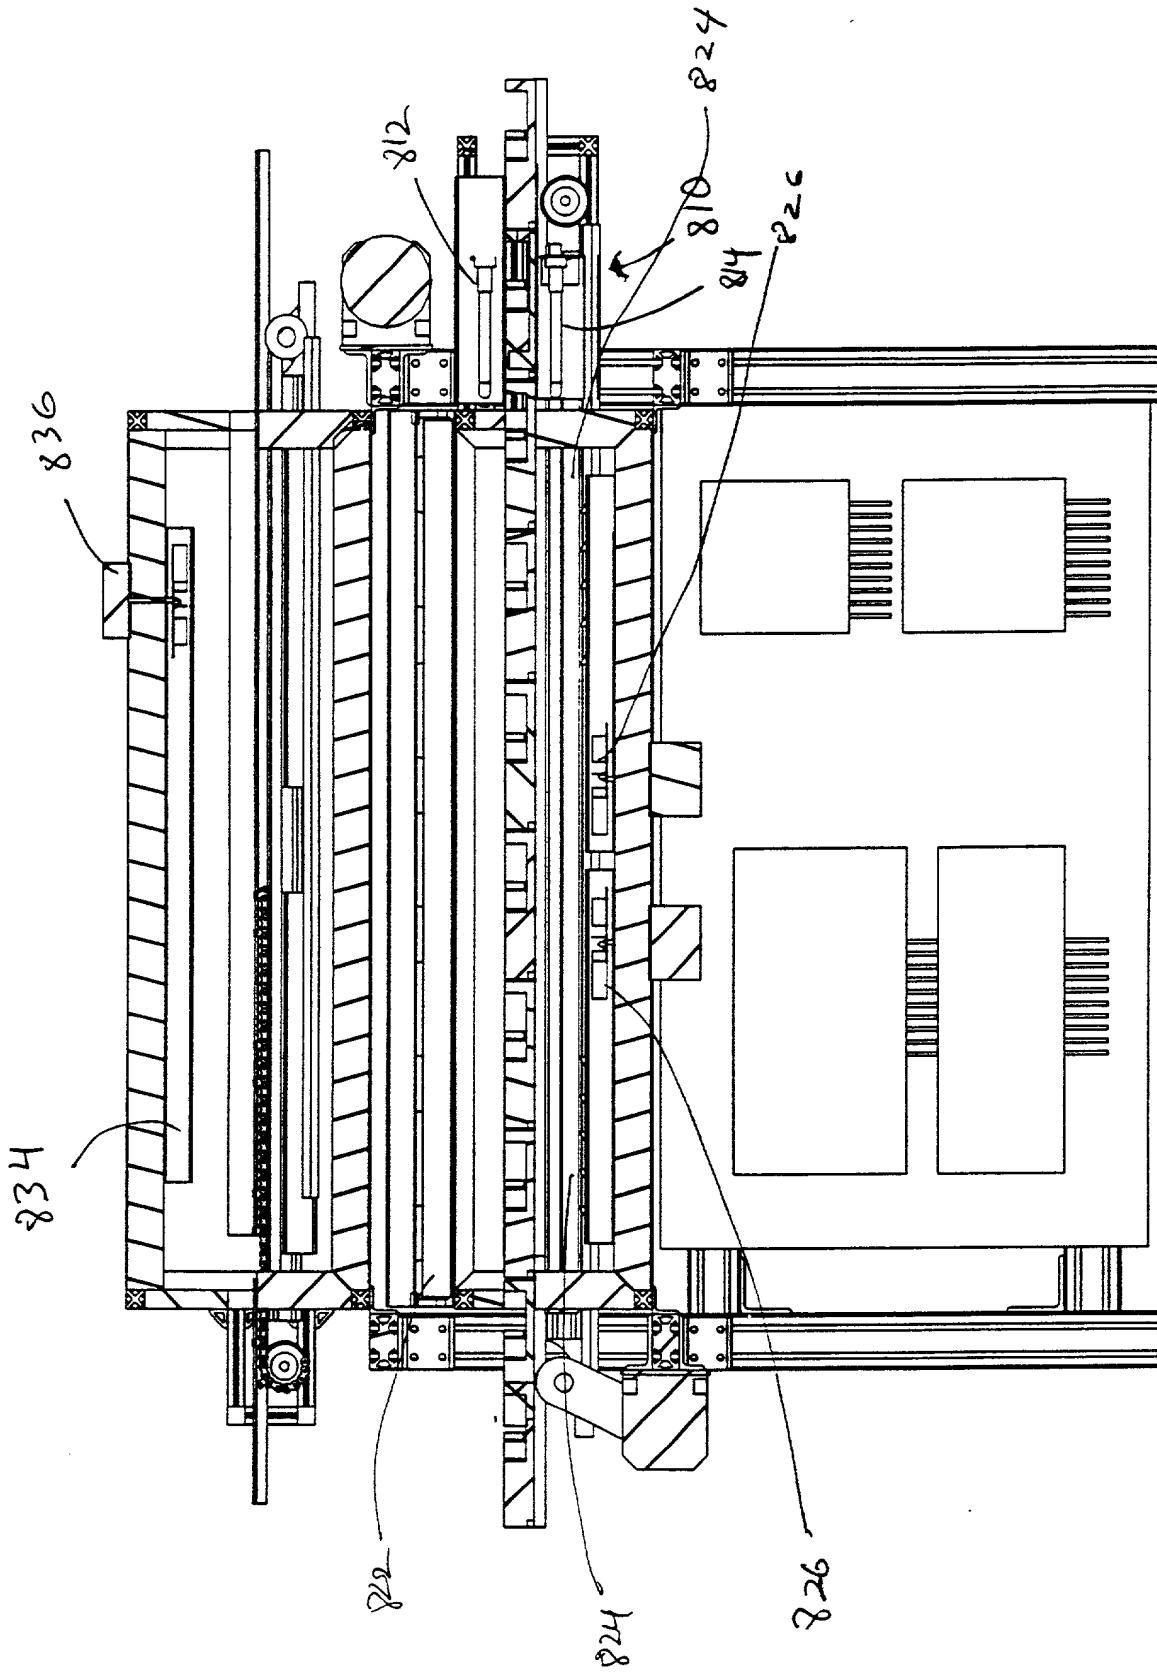


FIG 28

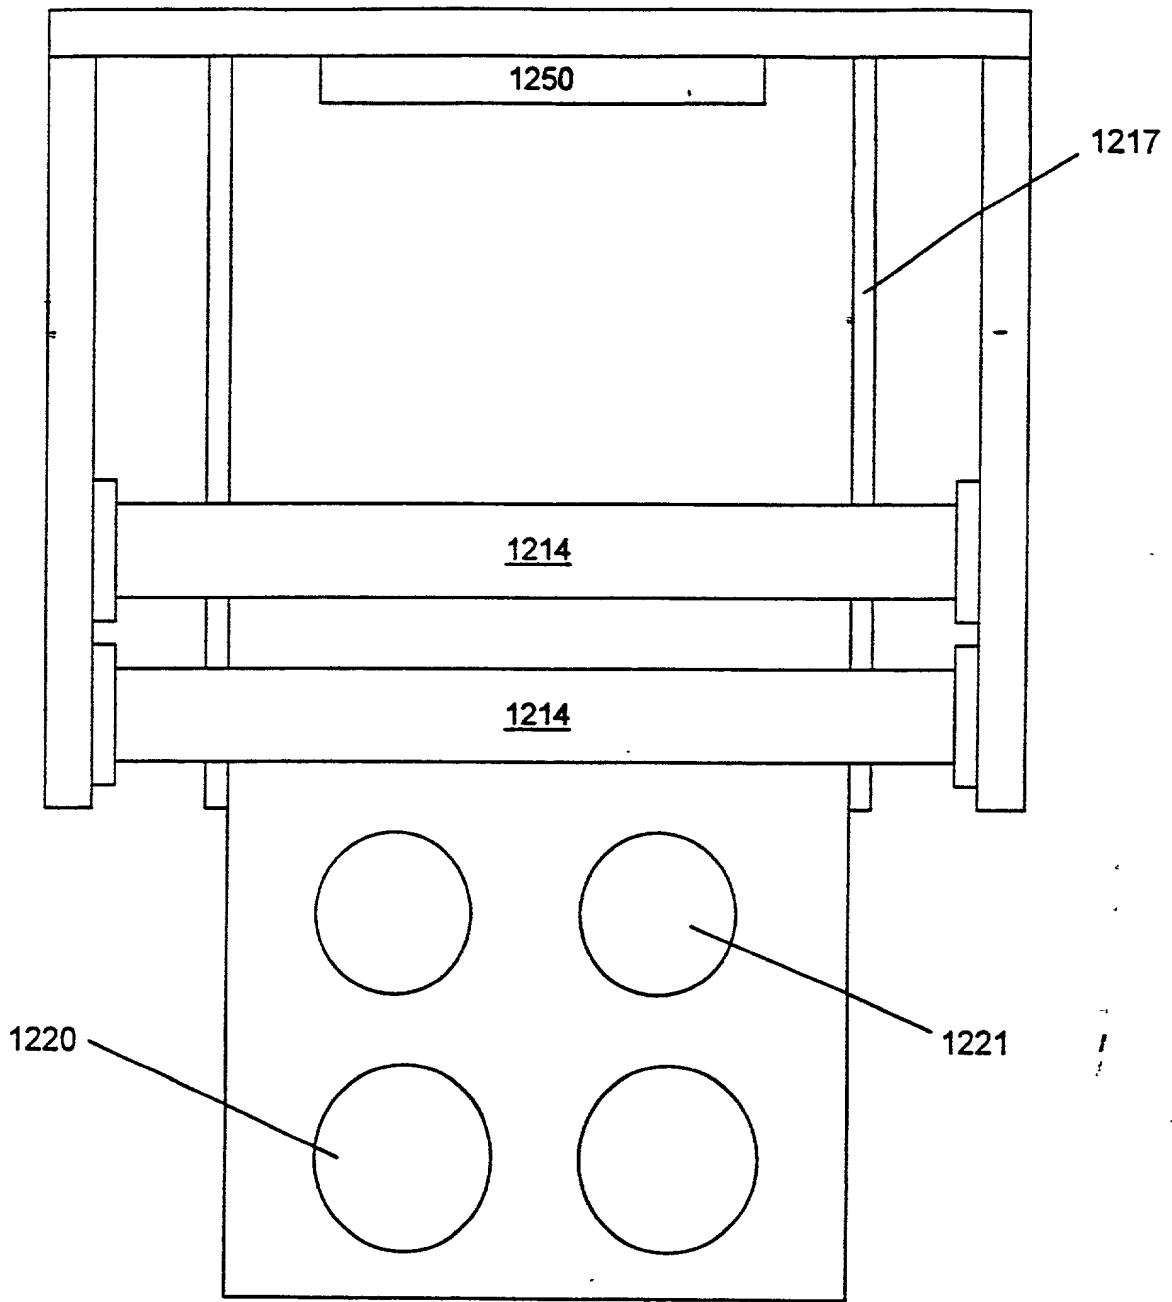


FIG. 26

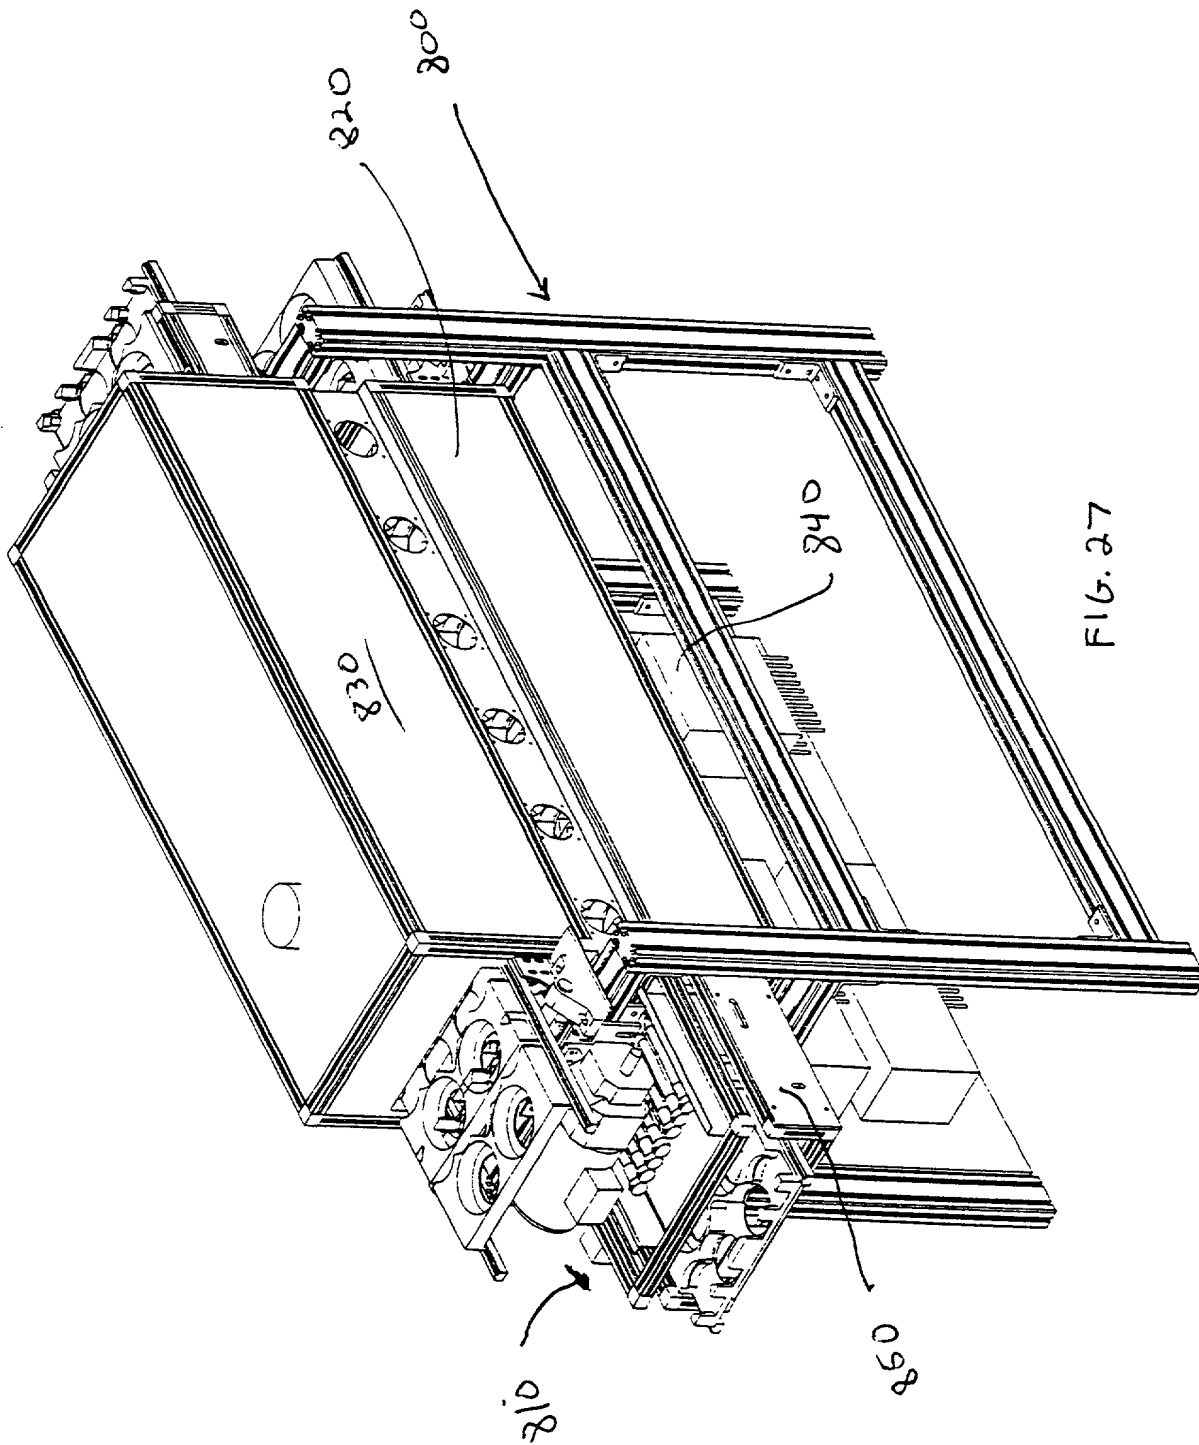


FIG. 27

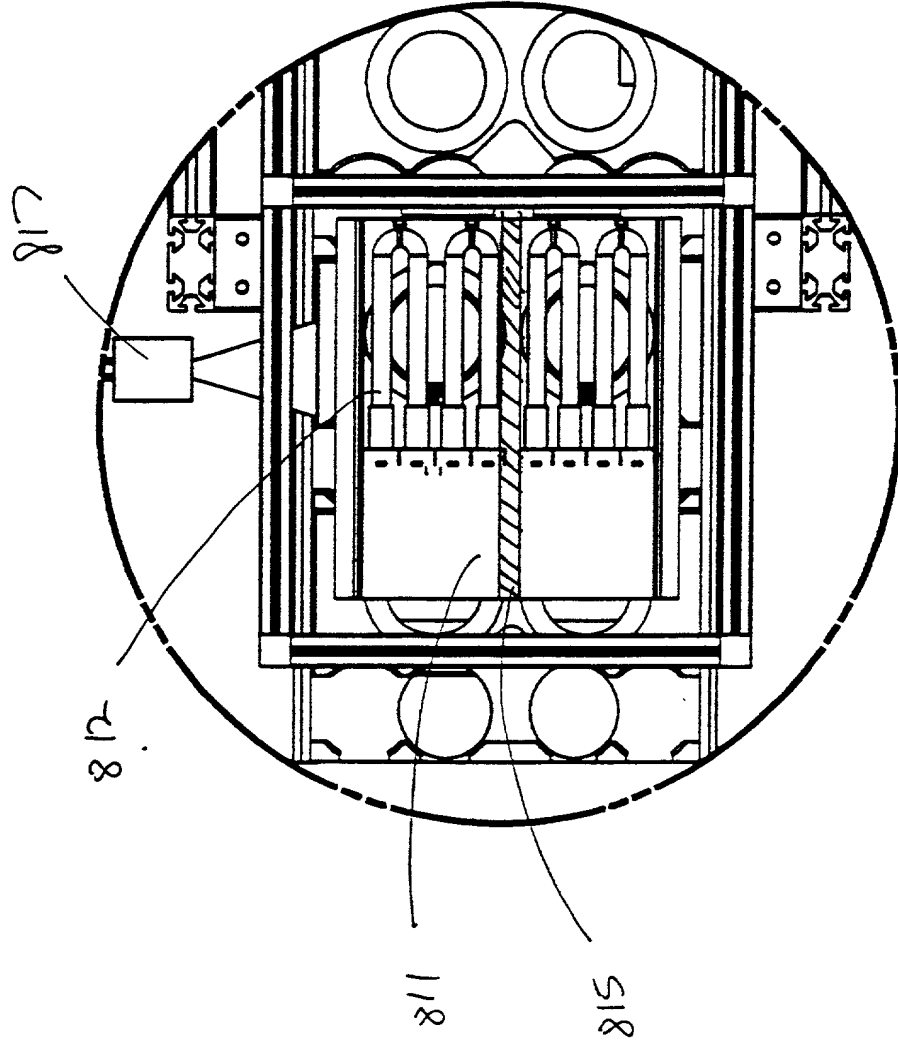


FIG. 29

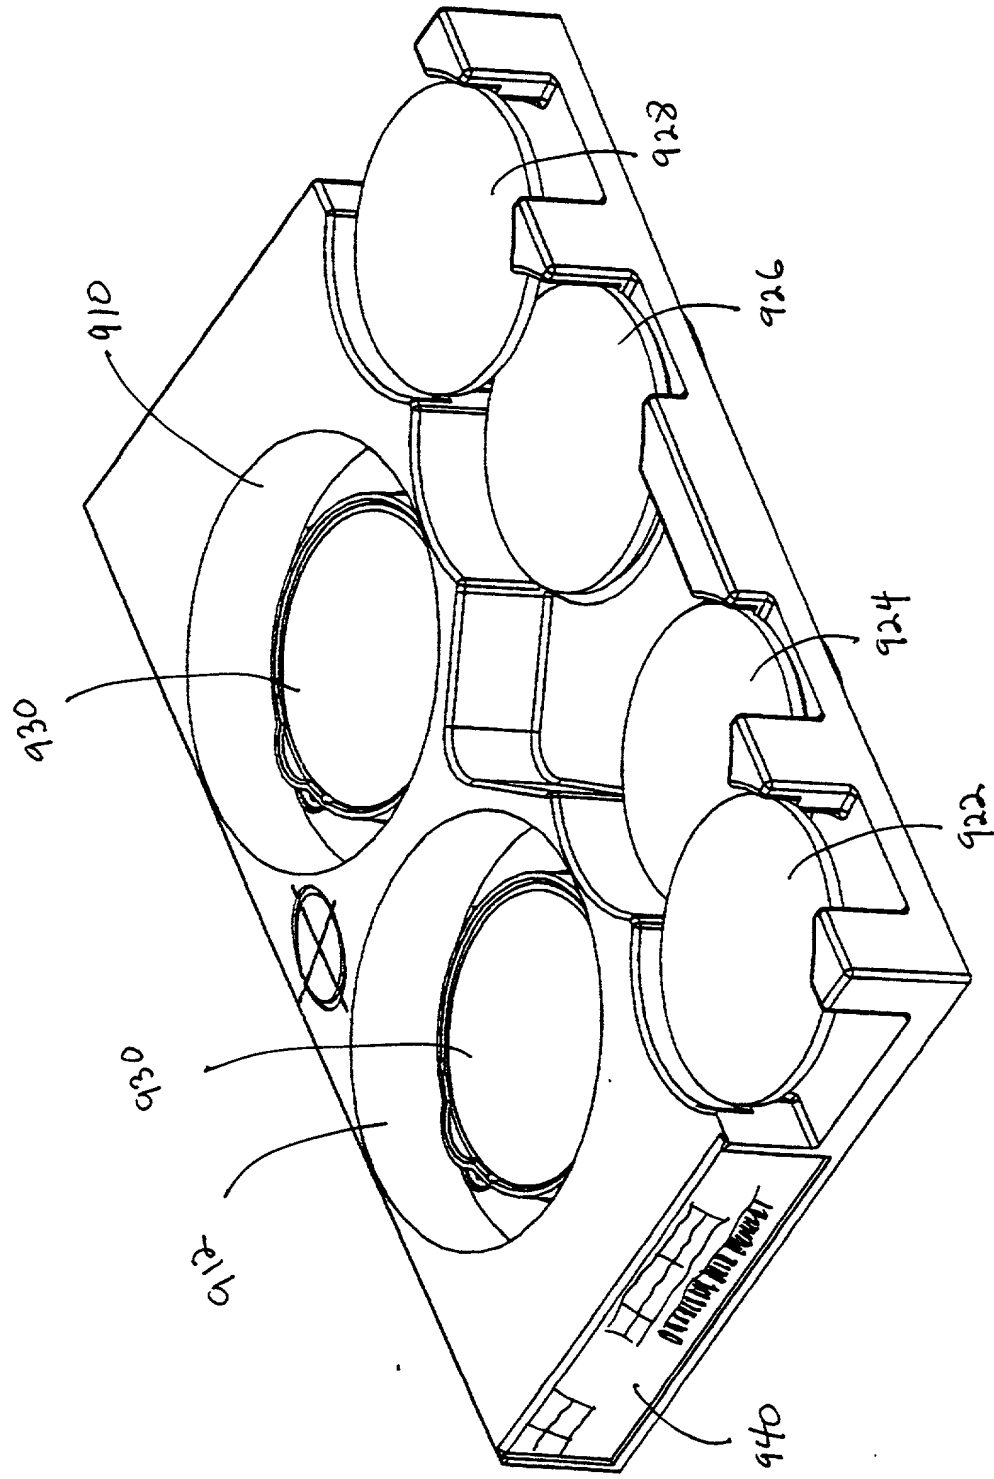


FIG. 30

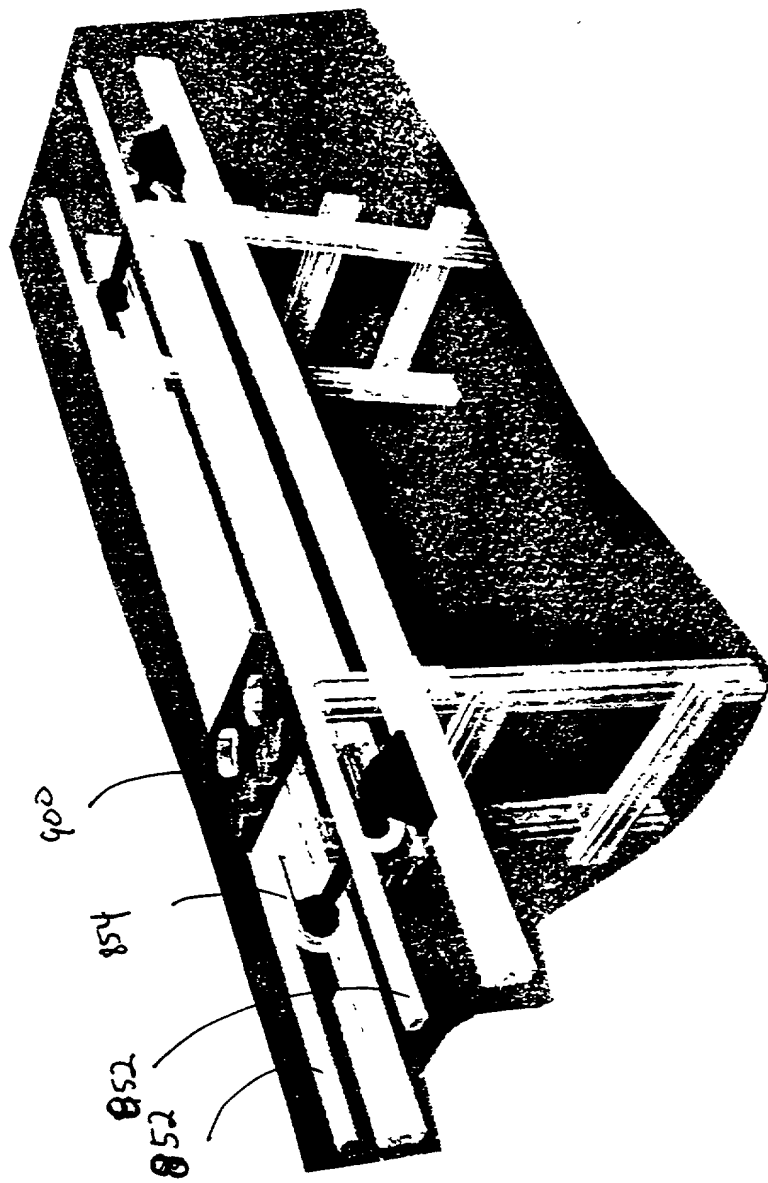


FIG. 31

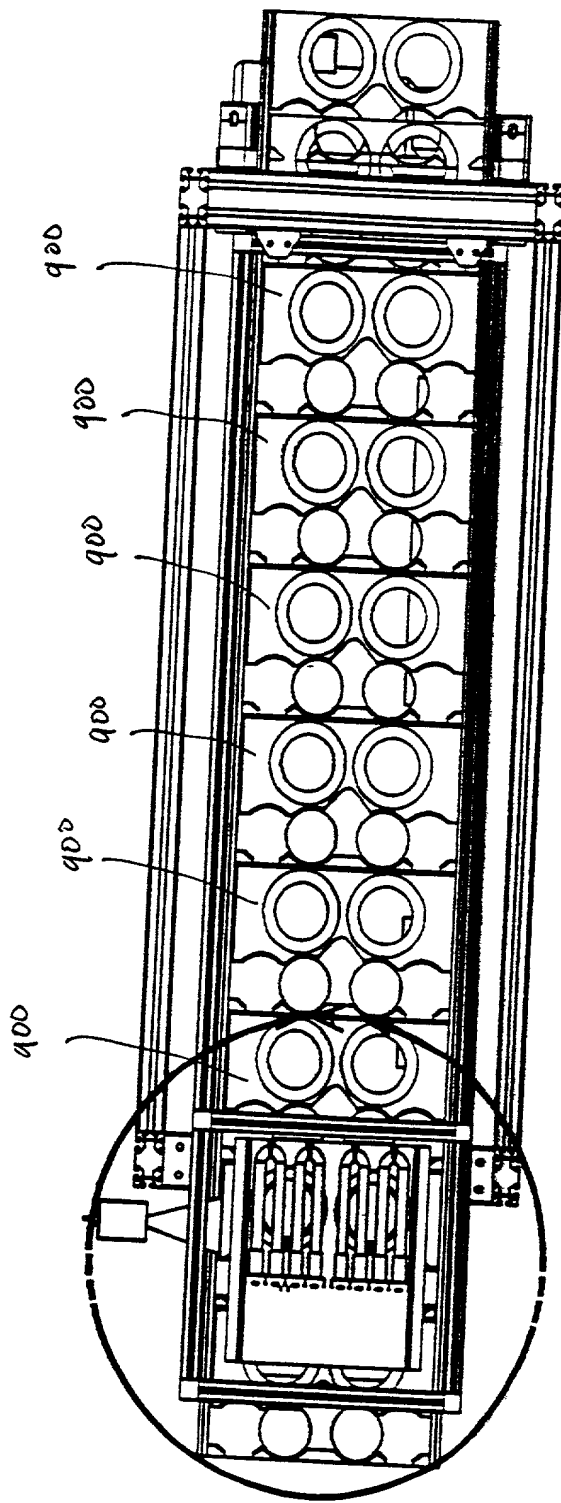


FIG. 32

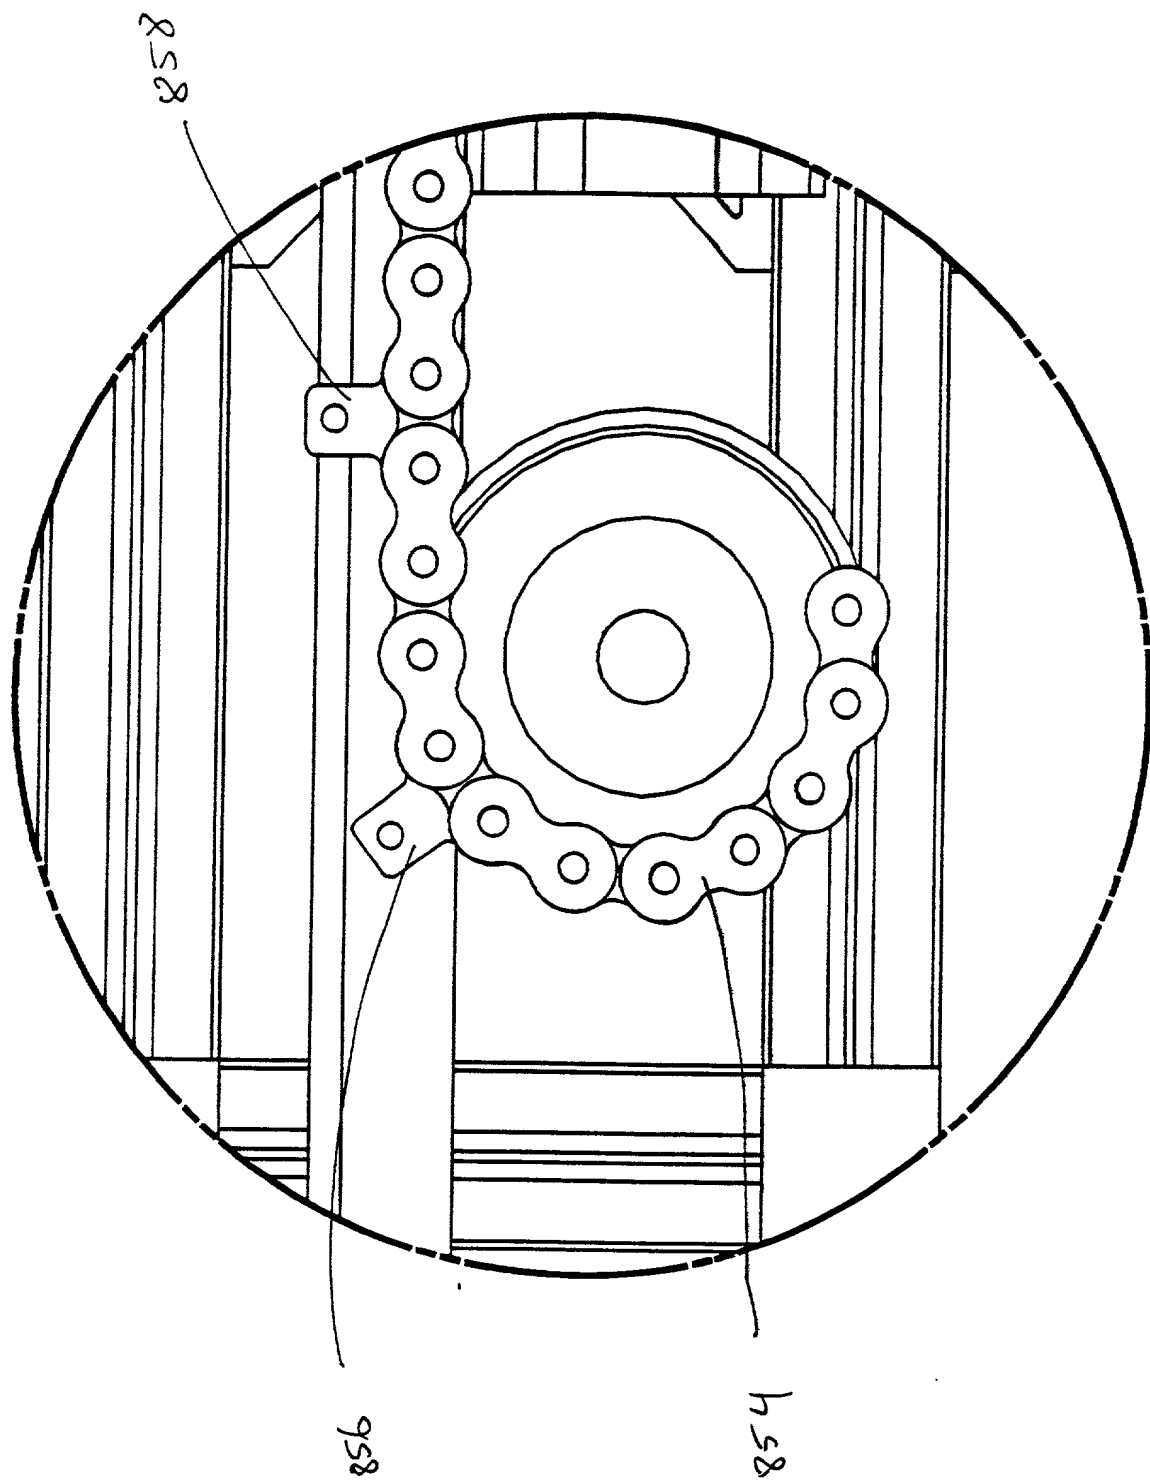


FIG. 33

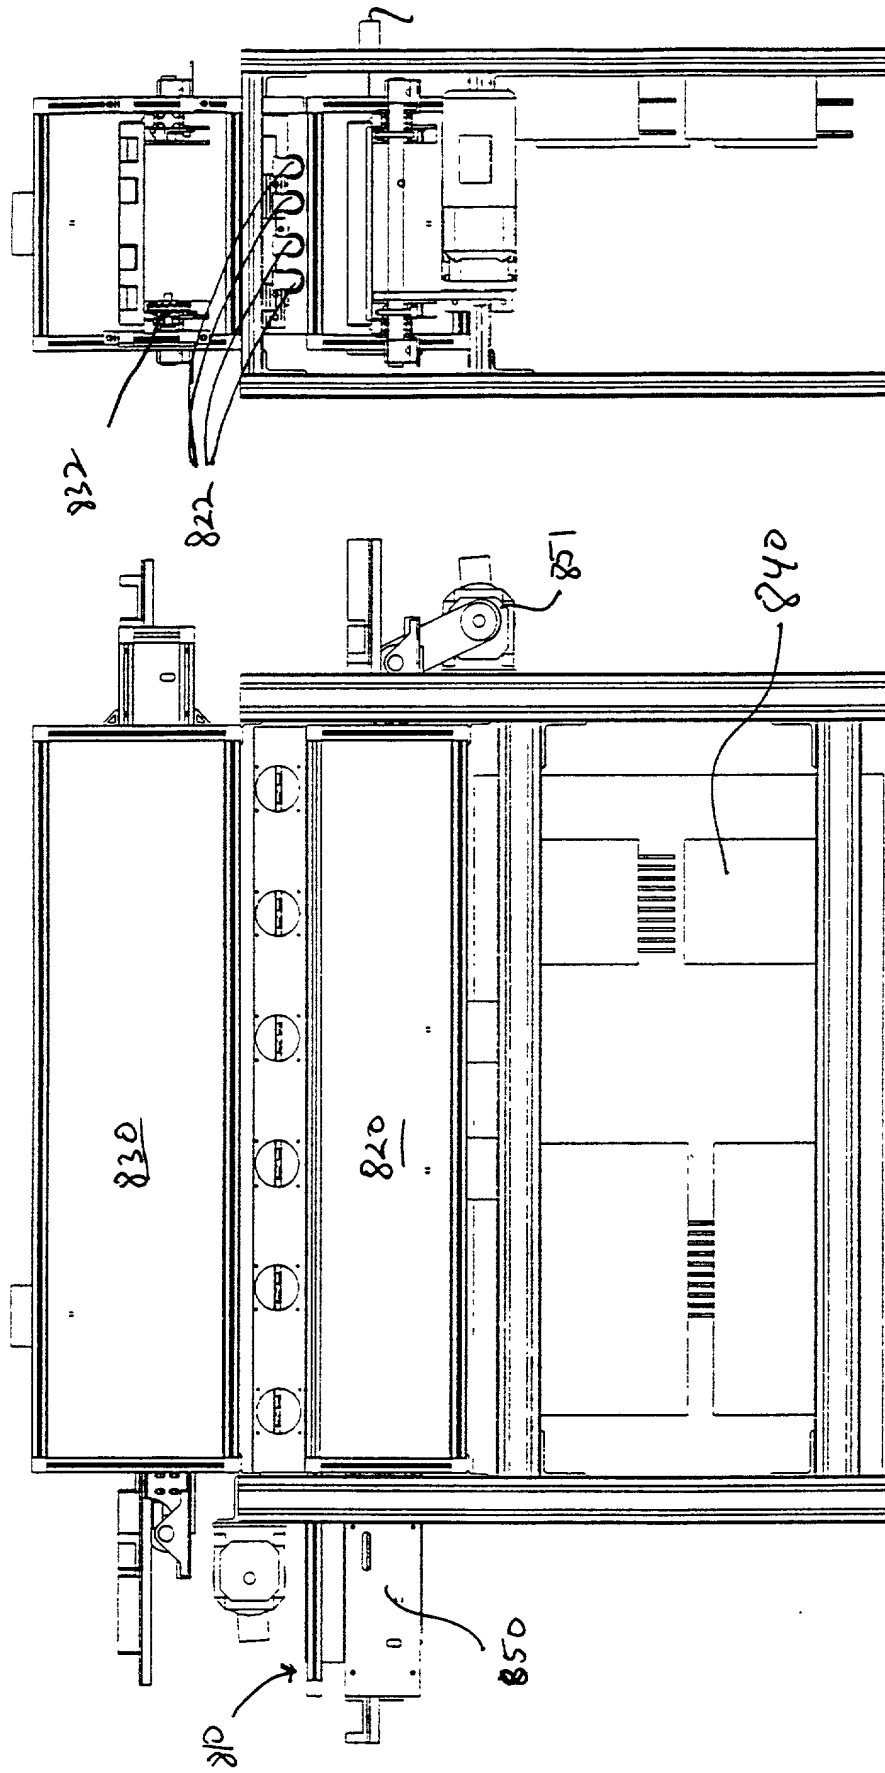


FIG. 34

FIG. 35



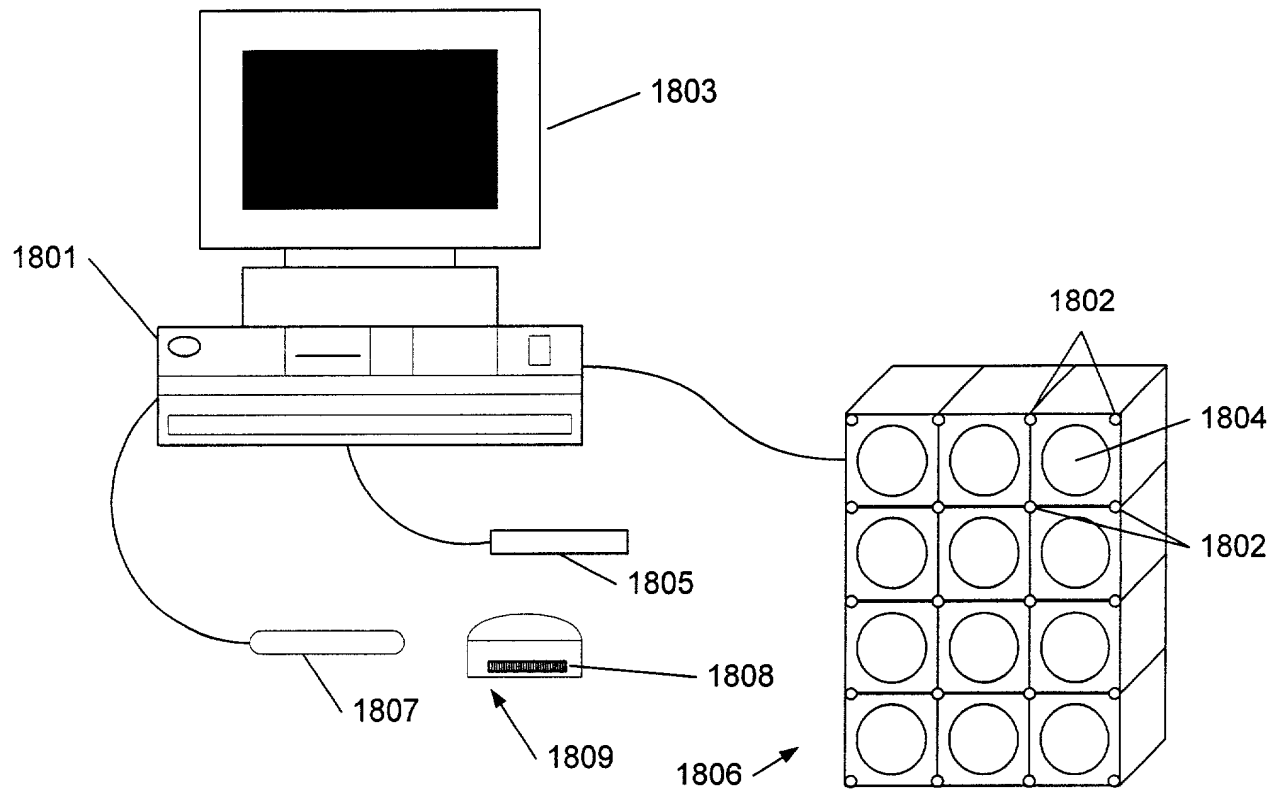


Fig.36

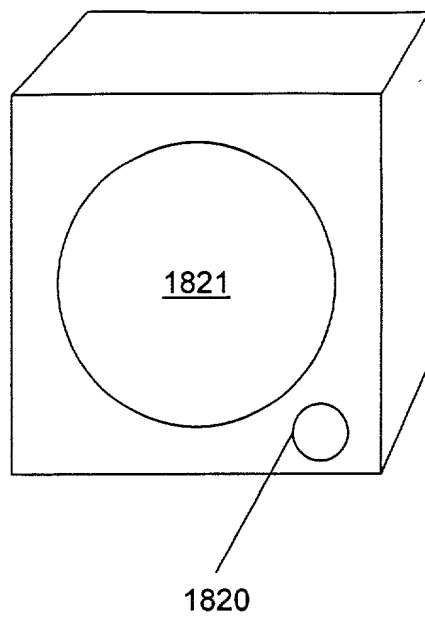

(a)

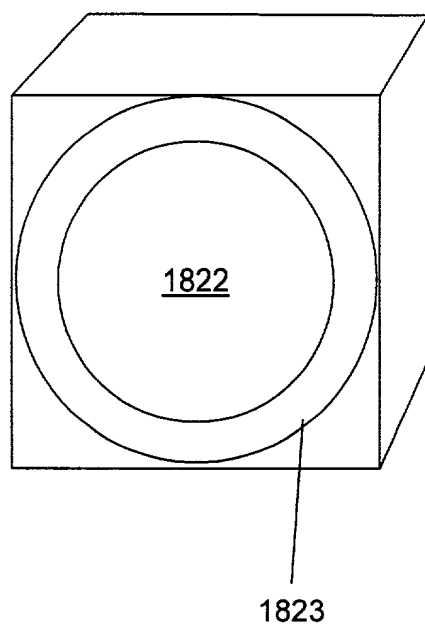

(b)

Fig. 37

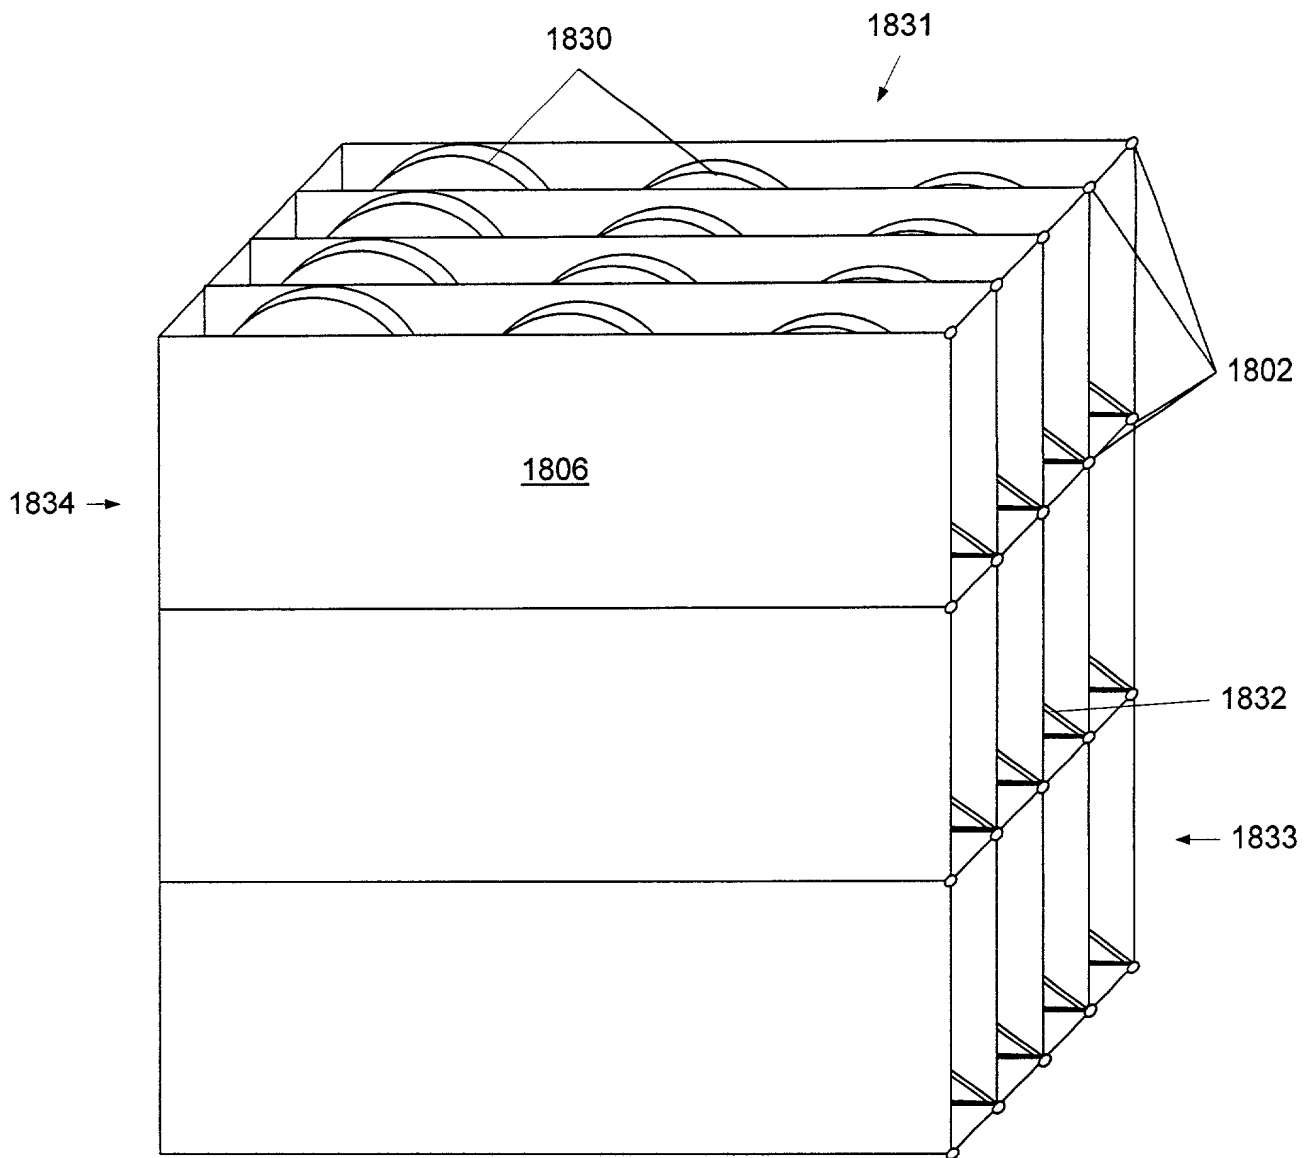


Fig. 38

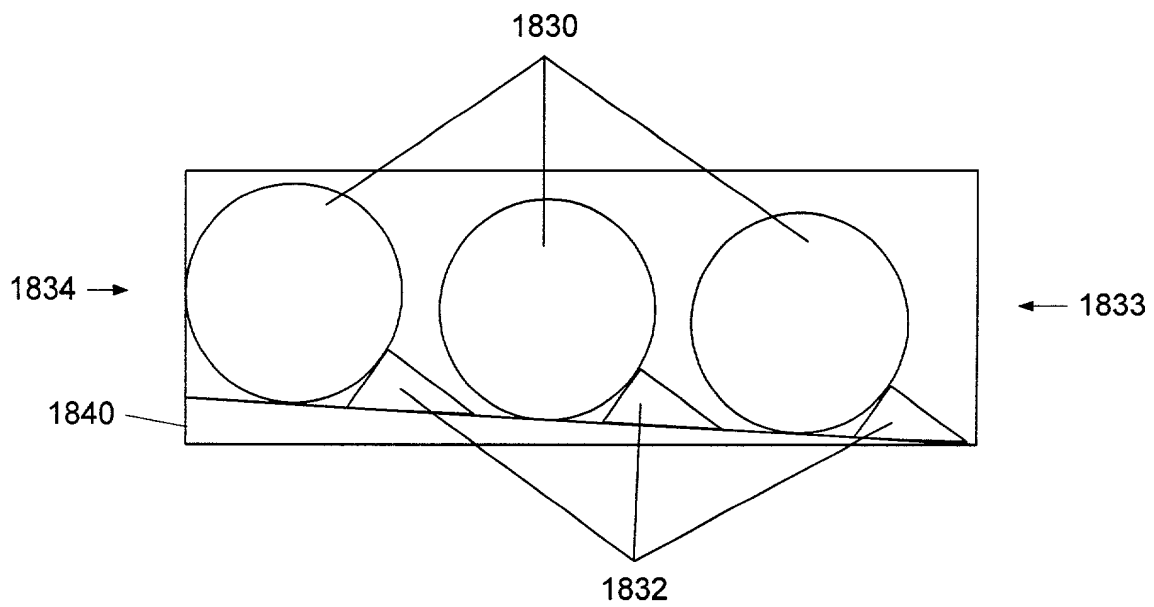


Fig. 39

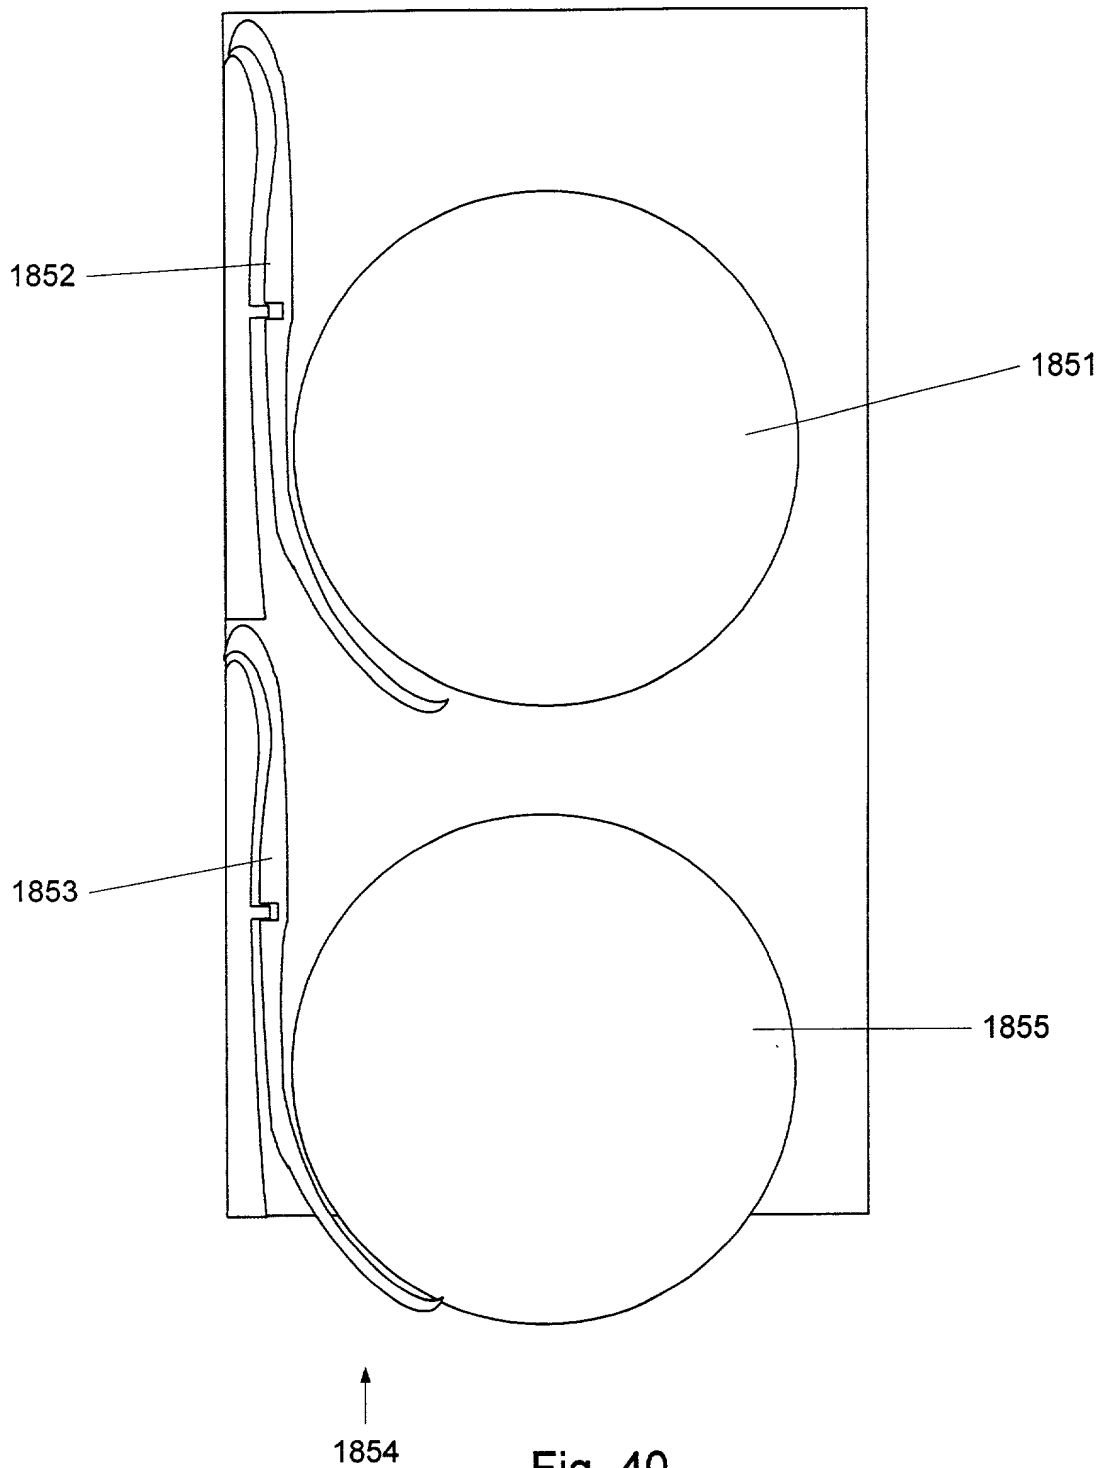


Fig. 40

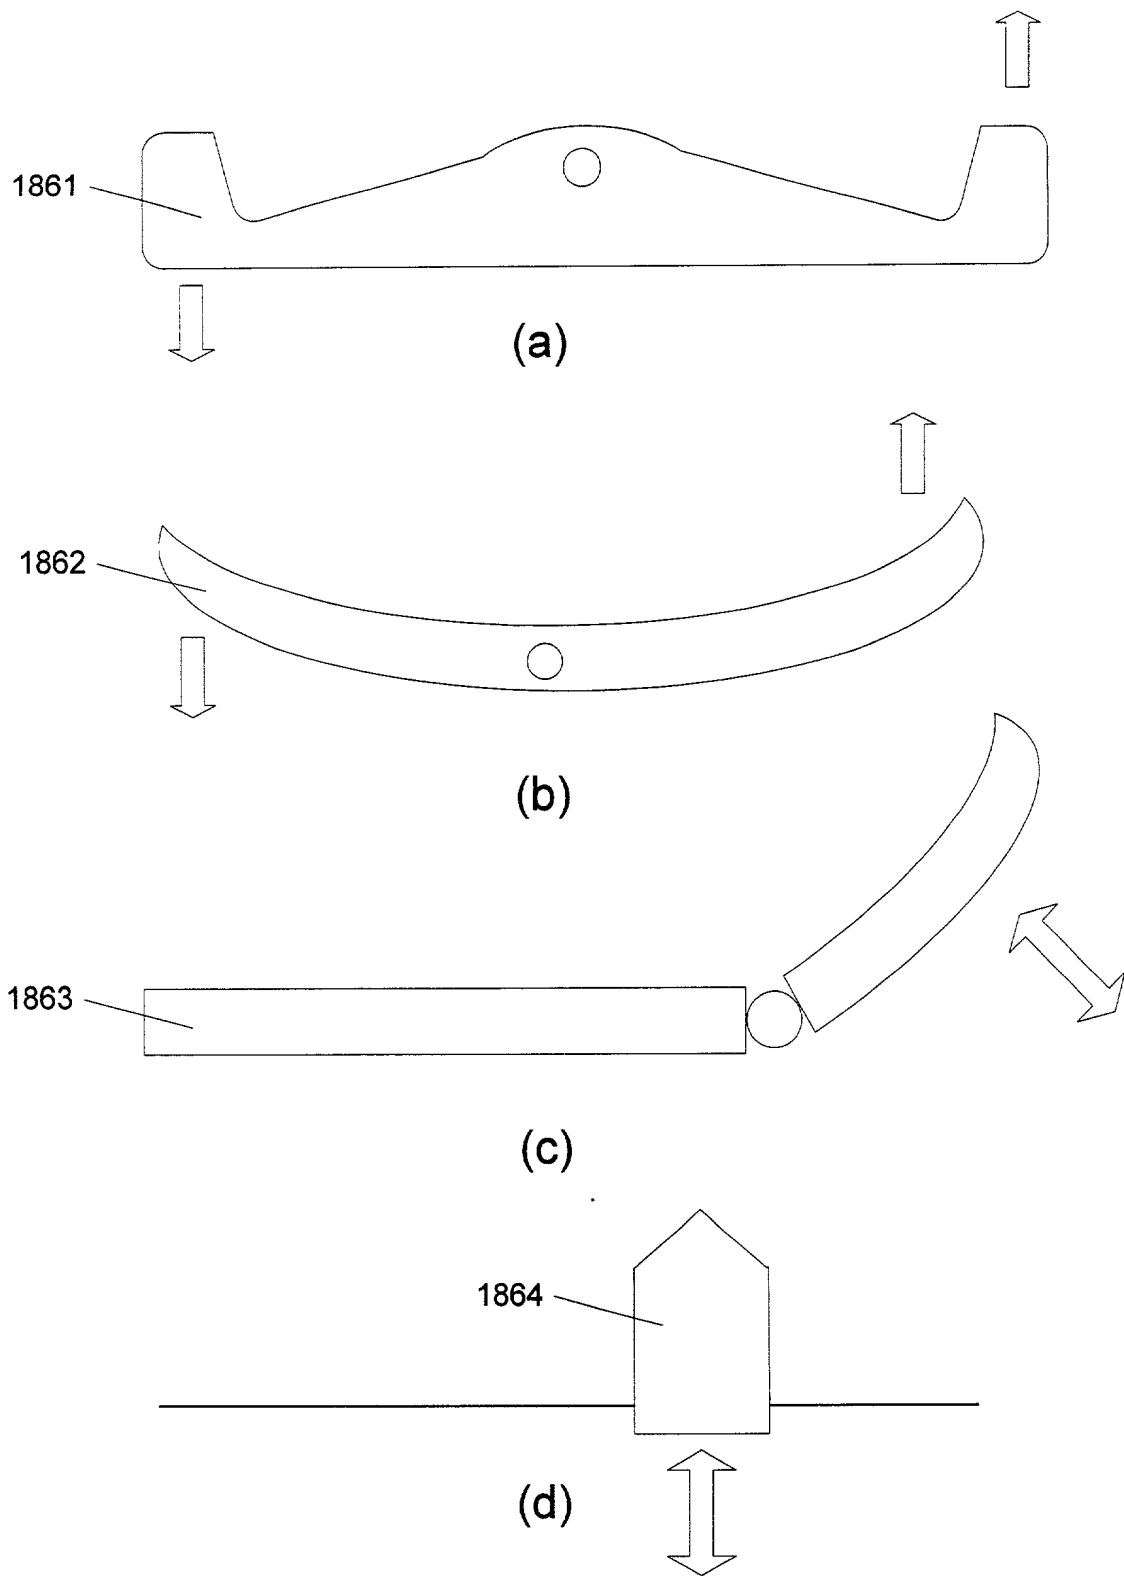


Fig. 41

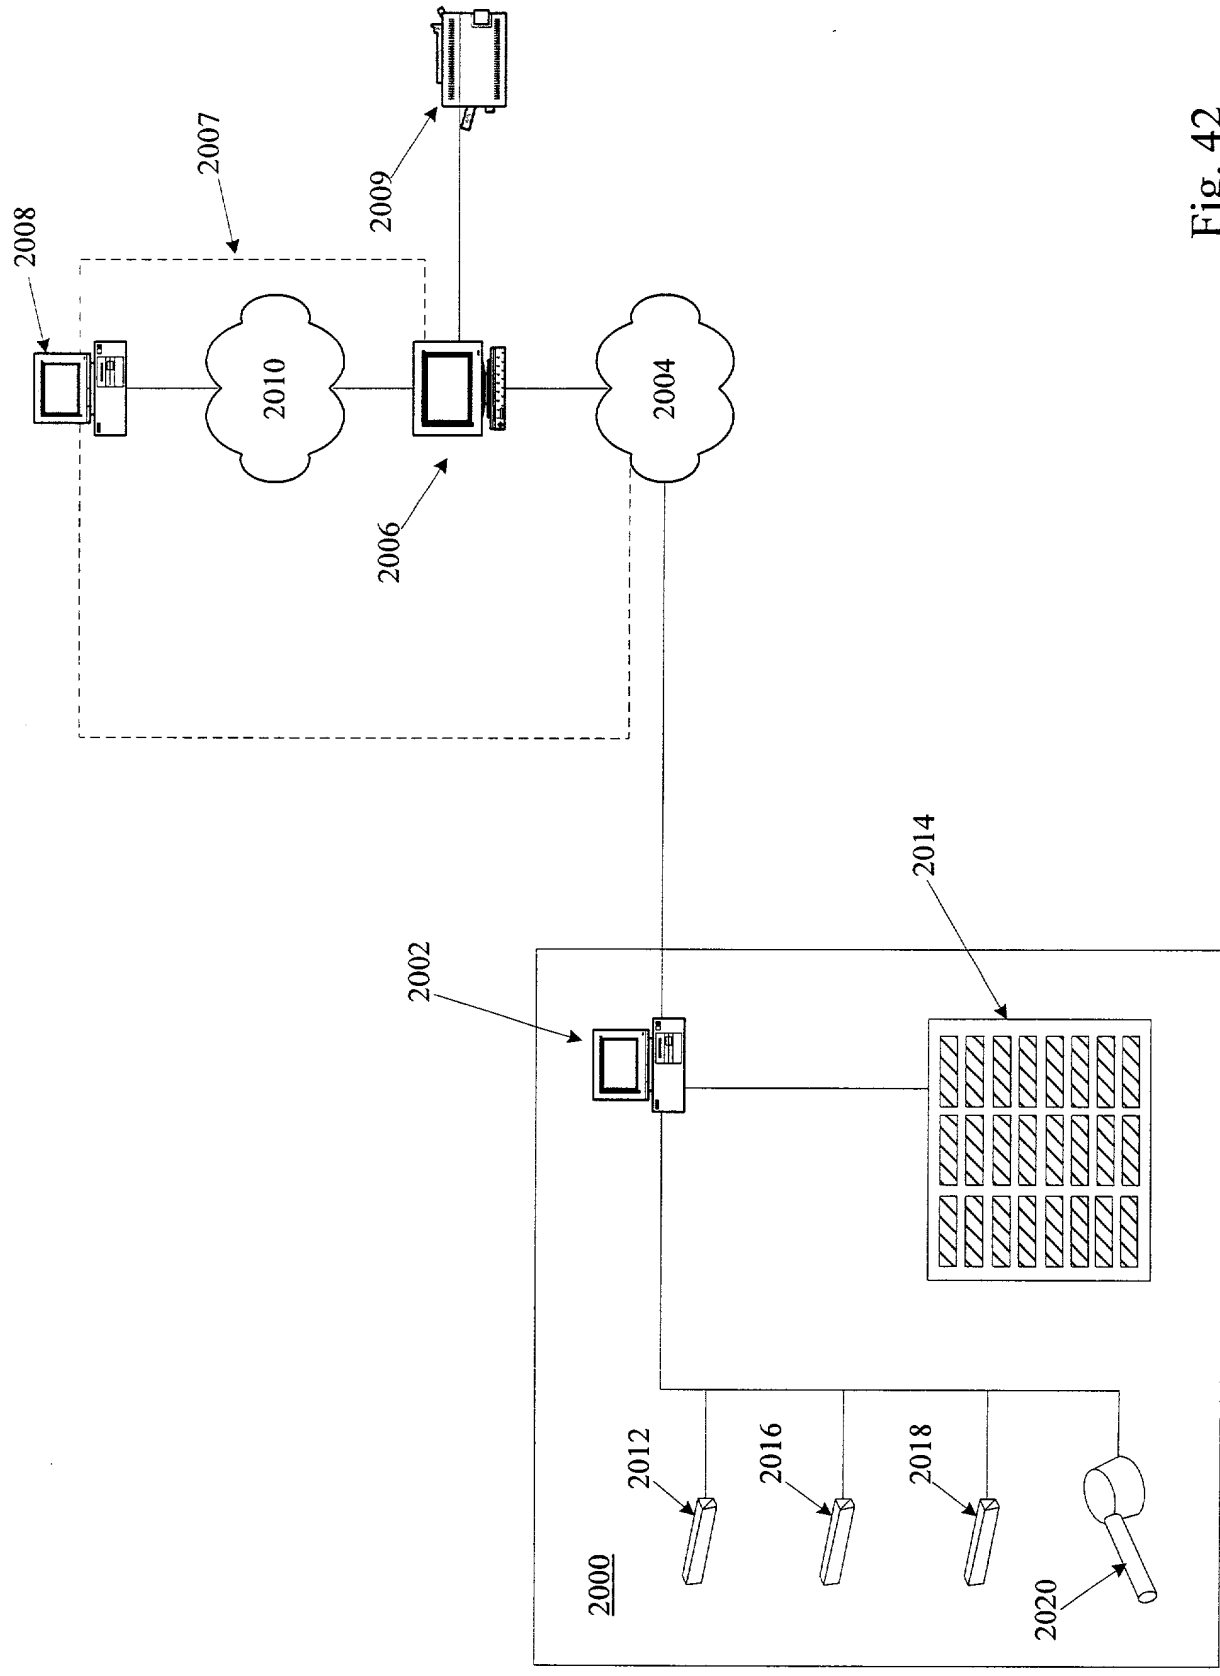


Fig. 42

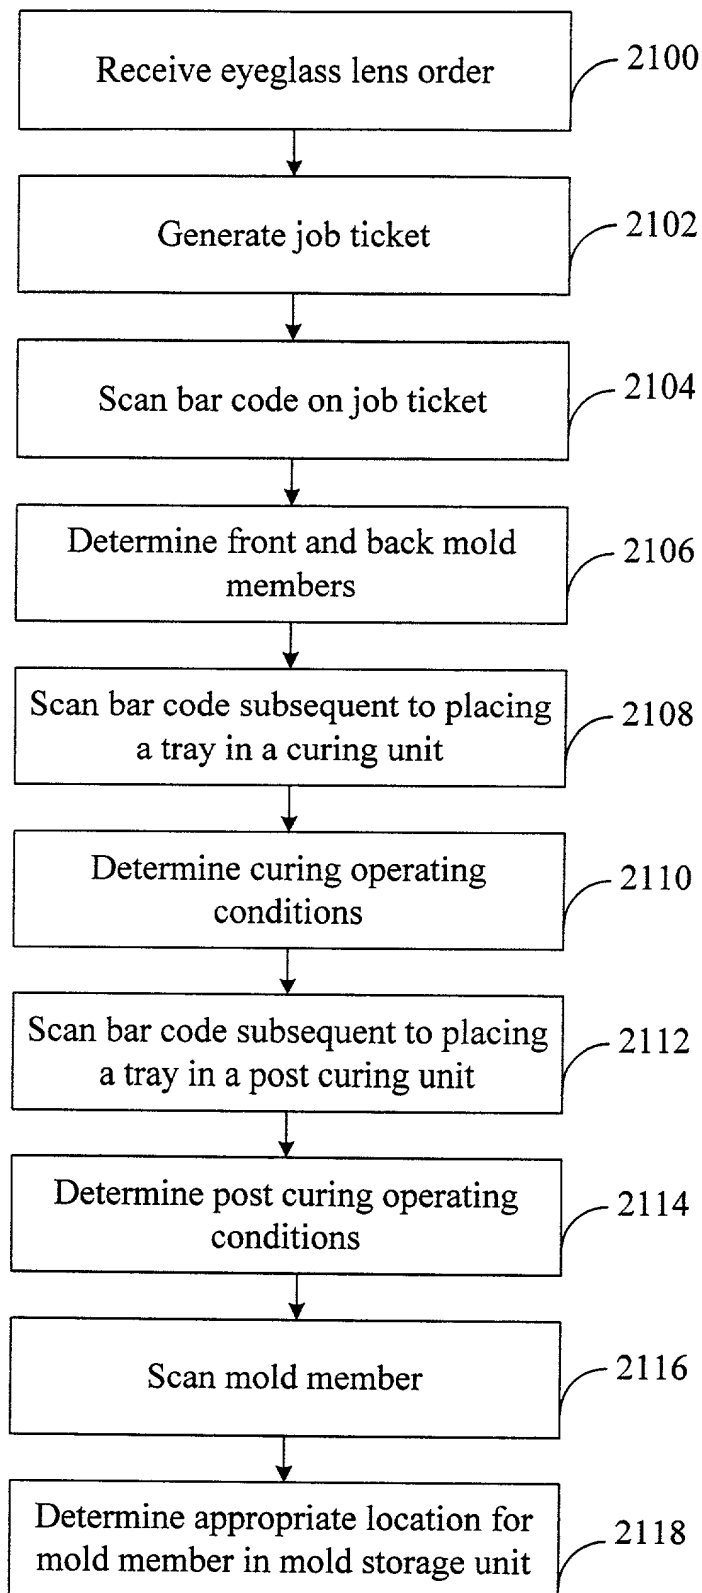


Fig. 43

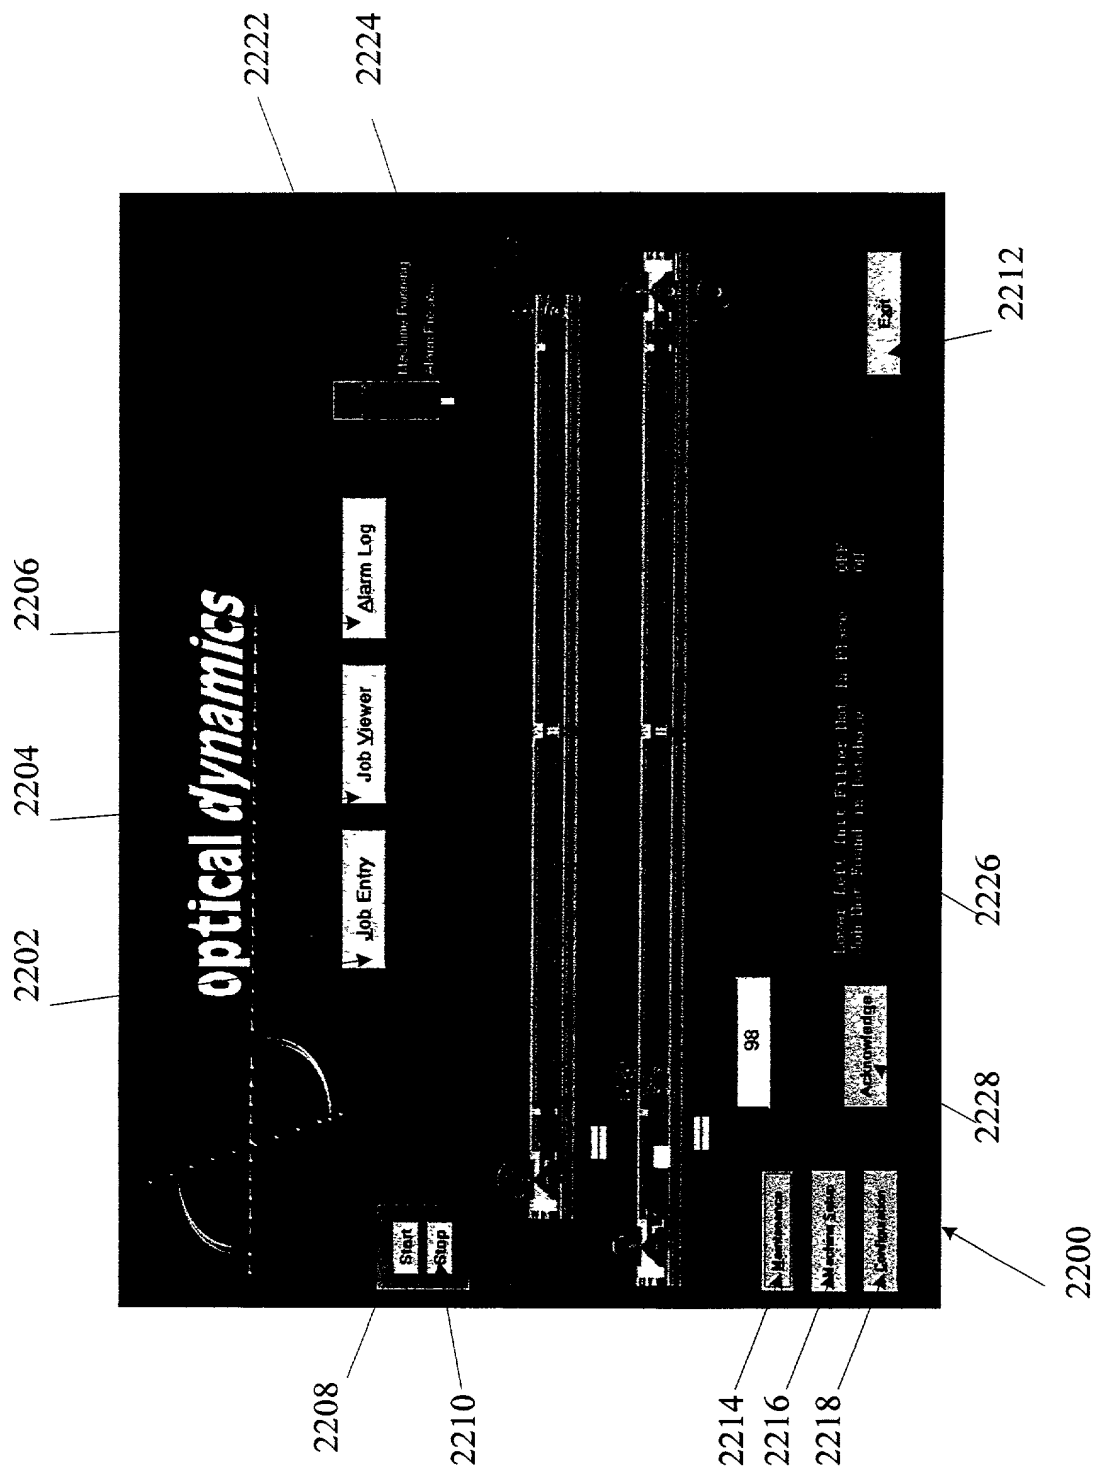


Fig. 44

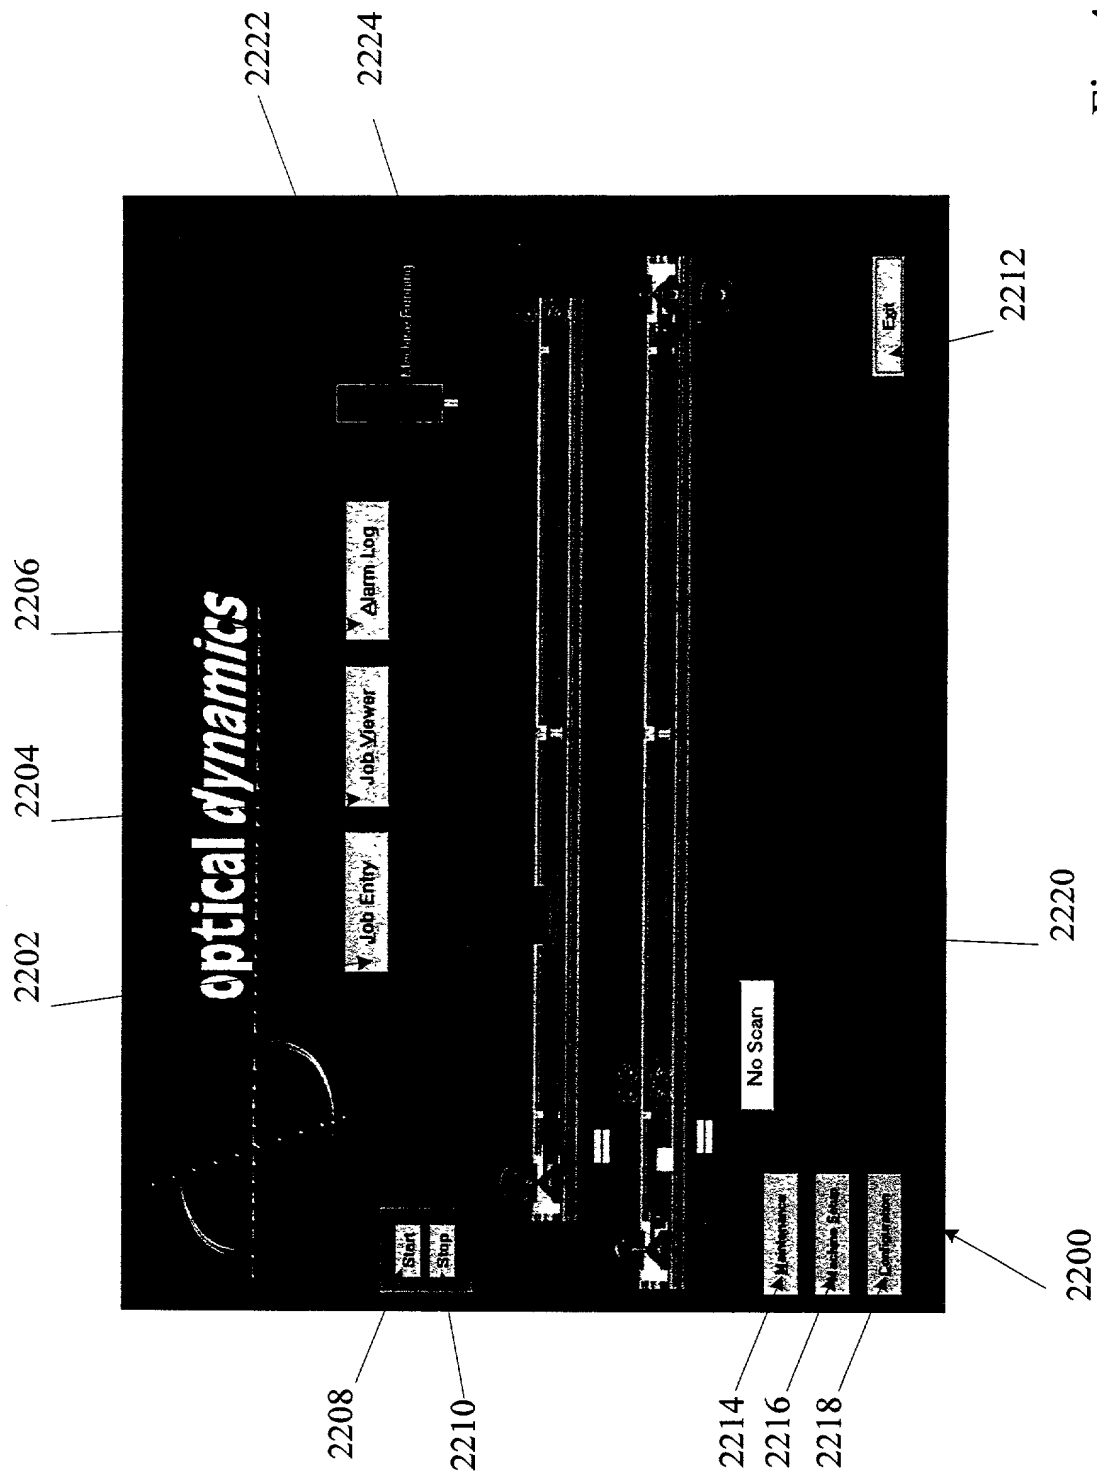


Fig. 45

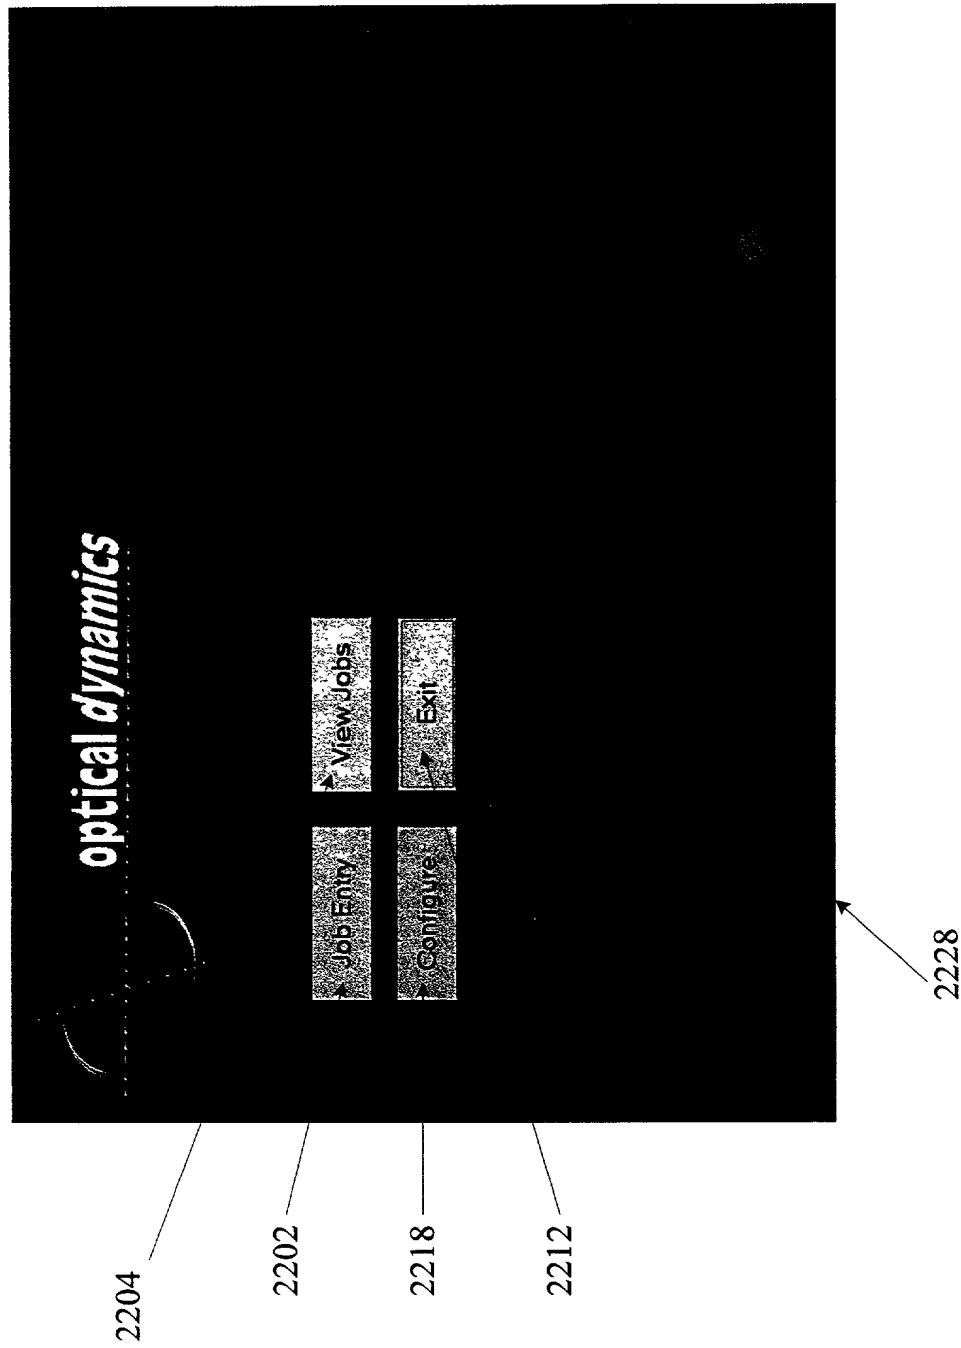


Fig. 46

Job Entry

Job # Patient Name 2232

Tray #

Bin Location

Priority ☐ Normal ☒ Re-Work ☐

Job Type

Right & Left Lens ☒ Aspheric - Single Vision ☒ Monomer/Tint ☐ Clear ☐ Clear w/ Tint ☐ Grey ☐

Right Lens Only ☐ Flat Top ☐ Paradigm Progressive ☐

Left Lens Only ☐

Right Eye

Sphere Cylinder

Left Eye

Sphere Cylinder

Cancel Entry Create Job 2238 2240

2234 2236 2230

Fig. 47

Job Viewer

LMS Job #

Patient

Entry Date

Lens Type

Monomer

LMS Tray #

Bin Location

Rx

Transposed

	Left	Right
Power	<input type="text" value="-6.00"/>	<input type="text"/>
Cylinder	<input type="text" value="-2.00"/>	<input type="text"/>
Axis	<input type="text"/>	<input type="text"/>
Add	<input type="text"/>	<input type="text"/>

Molds

	Left	Right
Front	<input type="text" value="No"/>	<input type="text"/>
Back	<input type="text" value="Rx"/>	<input type="text"/>
Gasket	<input type="text" value="Mold"/>	<input type="text"/>
Filter	<input type="text"/>	<input type="text"/>
Recipe	<input type="text"/>	<input type="text"/>

Re-Print

Close

Fig. 48

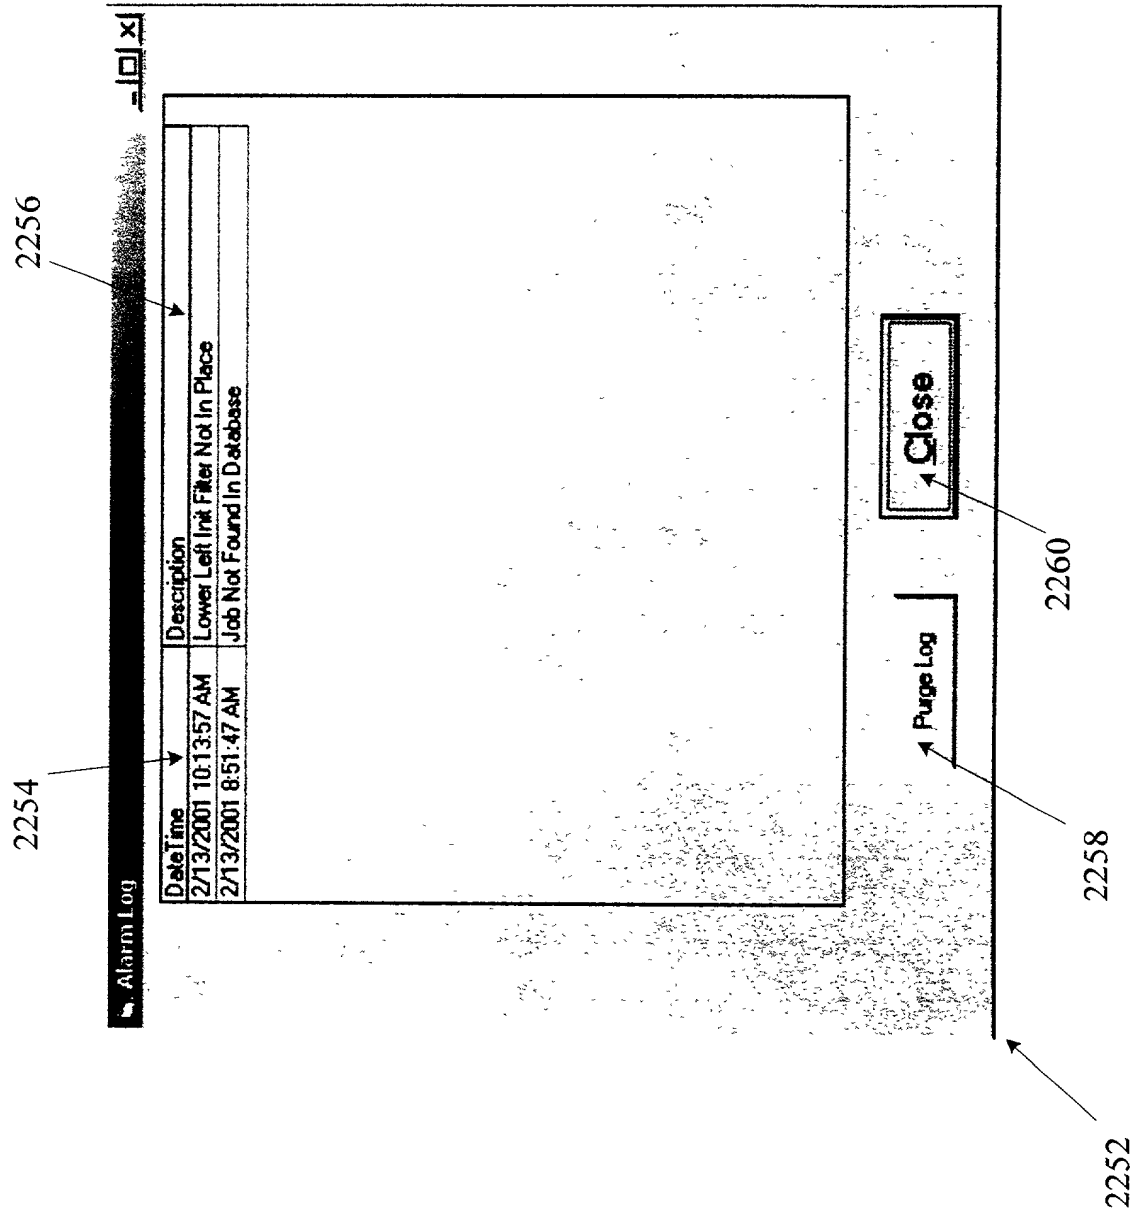


Fig. 49

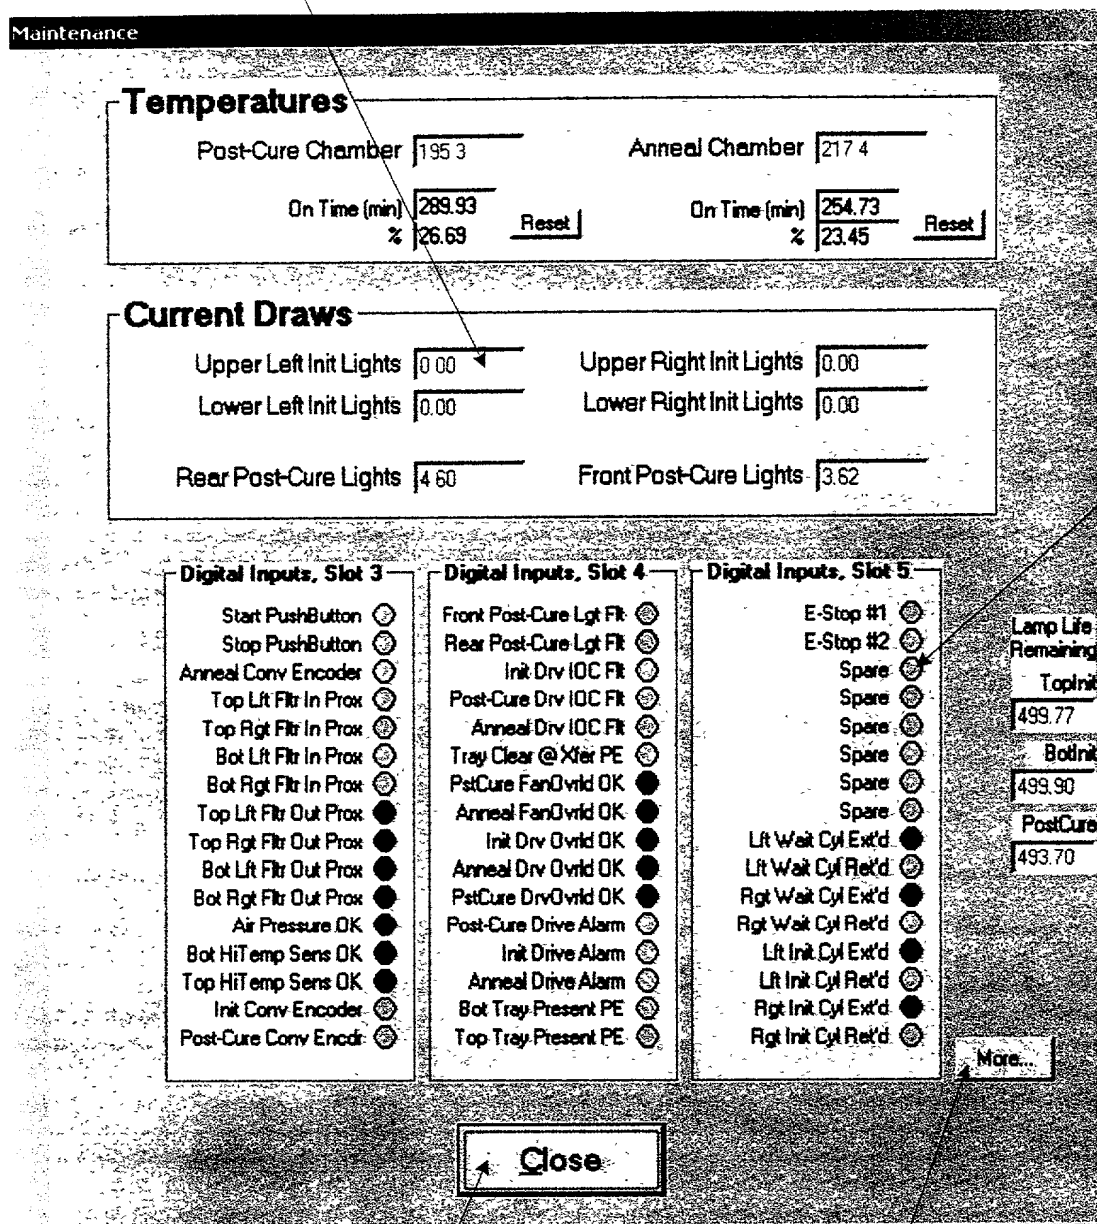


Fig. 50

Machine Setup

Anneal Conveyor

High Temp Alarm Limit

Temperature Setpoint

Low Temp Alarm Limit

Post-Cure Conveyor

High Temp Alarm Limit

Temperature Setpoint

Low Temp Alarm Limit

Initialization Lights

High Current Alarm Limit

Low Current Alarm Limit

No Scan Upper Init Time

No Scan Lower Init Time

No Scan Filter Select ☐

Post-Cure Lights

High Current Alarm Limit

Low Current Alarm Limit

Lamp Maintenance

Replaced Top Init Lamps ☐

Replaced Bot Init Lamps ☐

Replaced Post-Cure Lamps ☐

Save Changes **Cancel Changes**

2274

2272

2278

2280

2276

Fig. 51

2282

Recipe DB: [C:\OptDyn\MGR112700.mdb] Browse... 2284 2286 2288

Job DB: [C:\OptDyn\Job Tickets.mdb] Browse... 2290

Ticket Dir: [C:\OptDyn\] Browse... 2292

Ticket Poll Rate (sec) [2] 2294

Ticket Print Scale (%) [100]

Archive Jobs Every [14] Days Keeping [3] Days

Cancel OK

Fig. 52

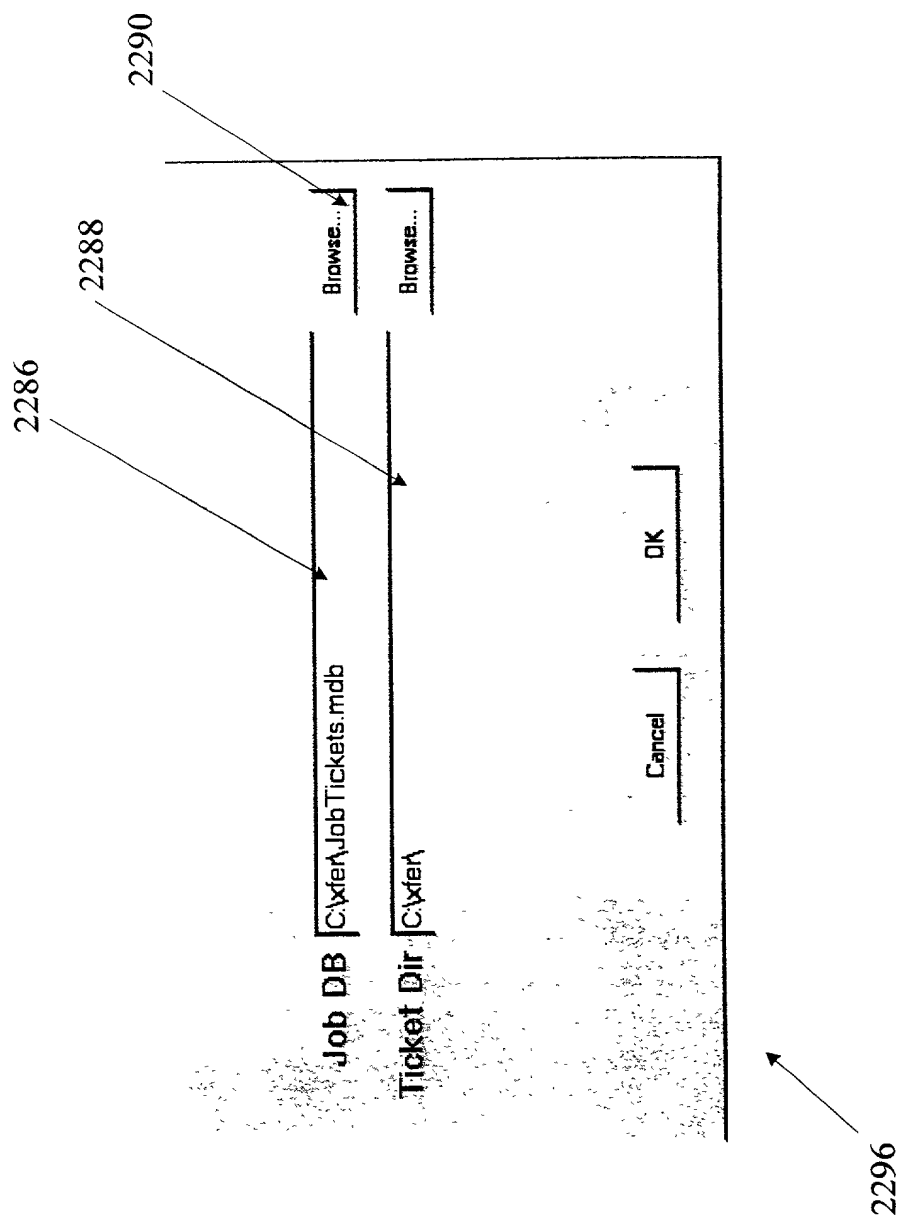


Fig. 53